



**TELEDYNE TEST TOOLS**  
Everywhereyoulook™



**Programming Manual  
Arbitrary Waveform Generator  
True-Arb Operating Mode  
High Definition AWG  
T3AWG3K Series  
Rev. 2.0**

## TABLE OF CONTENTS

<b>1. PREFACE.....</b>	<b>9</b>
1.1 ABBREVIATIONS AND TERMS .....	9
<b>2. REVISION HISTORY .....</b>	<b>10</b>
<b>3. SYNTAX AND COMMANDS .....</b>	<b>13</b>
3.1 COMMAND SYNTAX.....	13
3.1.1 Syntax Overview.....	13
3.1.2 Command and Query Structure .....	13
3.1.3 Command Entry .....	15
3.1.4 Parameter Types .....	16
3.1.5 SCPI Commands and Queries .....	19
<b>4. THE REGISTERS .....</b>	<b>20</b>
4.1 STATUS AND EVENTS.....	20
4.1.1 Status and event reporting system.....	20
4.1.2 Status Byte Register (SBR) .....	22
4.1.3 Service Request Enable Register (SRER).....	23
4.1.4 Standard Event Status Block (SESB) .....	23
4.1.5 Operation status block .....	24
4.1.6 Questionable status block.....	25
4.2 ANALOG DATA FORMAT (.TXT FILE ONLY).....	26
4.3 DIGITAL DATA FORMAT (.TXT FILE ONLY) .....	26
4.4 GRANULARITY .....	27
4.5 TRANSFERRING DATA FILE.....	27
4.5.1 Block Data Format .....	27
4.6 BYTE ORDER DURING TRANSFER .....	27
4.7 HOW TO GENERATE AN ARBITRARY WAVEFORM .....	28
<b>5. COMMAND GROUPS .....</b>	<b>29</b>
5.1 CONTROL GROUP COMMANDS .....	29
5.2 CALIBRATION AND DIAGNOSTIC COMMANDS .....	30
5.3 OUTPUT GROUP COMMANDS .....	30
5.4 DISPLAY COMMANDS .....	31
5.5 LICENSE COMMANDS.....	31
5.6 MARKER COMMANDS.....	32
5.7 CLOCK GROUP COMMANDS .....	32
5.8 IEEE MANDATED AND OPTIONAL GROUP COMMANDS .....	33
5.9 PARAMETRIC WAVEFORMS COMMANDS .....	33
5.10 STATUS GROUP COMMANDS.....	35
5.11 SYSTEM GROUP COMMANDS .....	36

5.12	MEMORY GROUP COMMANDS .....	37
5.13	MASS MEMORY COMMANDS .....	37
5.14	TRIGGER GROUP COMMANDS .....	39
5.15	SEQUENCE GROUP COMMANDS .....	39
5.16	WAVEFORM GROUP COMMANDS .....	41
5.17	MULTI INSTRUMENT COMMANDS .....	42
<b>6.</b>	<b>COMMAND DESCRIPTIONS .....</b>	<b>43</b>
6.1	CONTROL GROUP COMMANDS .....	43
6.2	CALIBRATION AND DIAGNOSTIC COMMANDS.....	52
6.3	OUTPUT GROUP COMMANDS .....	54
6.4	DISPLAY GROUP COMMANDS.....	60
6.5	LICENSE GROUP COMMANDS .....	63
6.6	MARKER GROUP COMMANDS .....	65
6.7	CLOCK GROUP COMMANDS .....	68
6.8	IEEE MANDATED AND OPTIONAL GROUP COMMANDS .....	70
6.9	PARAMETRIC WAVEFORMS COMMANDS .....	75
6.10	MEMORY GROUP COMMANDS .....	100
6.11	MASS MEMORY GROUP COMMANDS .....	105
6.12	STATUS GROUP COMMANDS.....	122
6.13	SYSTEM GROUP COMMANDS .....	126
6.14	TRIGGER GROUP COMMANDS .....	130
6.15	SEQUENCE GROUP COMMANDS .....	136
6.16	WAVEFORM GROUP COMMANDS .....	150
6.17	MULTI INSTRUMENT GROUP COMMANDS.....	157
<b>7.</b>	<b>COMMAND ERRORS .....</b>	<b>160</b>
<b>8.</b>	<b>PREDEFINED WAVEFORMS.....</b>	<b>162</b>
<b>9.</b>	<b>REMOTE CONTROL .....</b>	<b>163</b>
9.1	PREREQUISITE .....	163
9.1.1	AT Instrument Communicator .....	168
9.2	NI LABVIEW EXAMPLES.....	170
9.2.1	Continuous Mode .....	171
9.2.2	Burst Mode .....	173
9.2.3	Stepped Mode .....	175
9.2.4	Advanced Mode .....	177
9.2.5	Import an Arbitrary Waveform Generation .....	179
9.3	SCRIPT EXAMPLES .....	182
9.3.1	Continuous Mode .....	182
9.3.2	Stepped Mode .....	183
9.3.3	Import Arbitrary.....	184

9.3.4 Advanced Mode ..... 185

**LIST OF TABLES**

Table 1: Abbreviations and terms .....	9
Table 2: Revision History.....	12
Table 3: Syntax symbols and their meanings .....	13
Table 4: Message symbols and their meanings .....	14
Table 5: Message terminator and meaning .....	16
Table 6: Parameter types, their descriptions, and examples .....	17
Table 7: String symbol and meaning .....	17
Table 8: SI prefixes and their indexes .....	18
Table 9: Status Byte Register (SBR) .....	22
Table 10: Service Request Enable Register (SRER) .....	23
Table 11: Standard Event Status Register (SESR) .....	24
Table 12: Operation Condition Register (OCR) .....	25
Table 13: Models and available parameters.....	29
Table 14: Control group commands .....	30
Table 15: Calibration and Diagnostic group commands.....	30
Table 16: Output group commands .....	31
Table 17: Display group commands .....	31
Table 18: License group commands .....	32
Table 19: Marker group commands .....	32
Table 20: Clock group commands .....	32
Table 21: IEEE Mandatory group commands .....	33
Table 22: Parametric Waveforms Commands.....	35
Table 23:Status group commands .....	36
Table 24: System group commands .....	37
Table 25: Memory Group commands .....	37
Table 26: Mass Memory Group commands.....	38
Table 27: Trigger group commands.....	39
Table 28: Sequence group commands .....	41
Table 29: Waveform group commands .....	42
Table 30: Multi-Instrument group commands and their descriptions .....	42
Table 31: AWGControl:AFGSwitch.....	43
Table 32: AWGControl:BURST.....	43
Table 33: AWGControl:CONFigure:CNUMber? .....	44
Table 34: AWGControl:CONFigure:DNUMber.....	44
Table 35: AWGControl:DECreasing.....	45

Table 36: AWGControl:INCreasing.....	45
Table 37: AWGControl:LENGth:MODE .....	46
Table 38: AWGControl:RESET[:IMMediate] .....	47
Table 39: AWGControl:RMODe .....	48
Table 40: AWGControl:RSTATe? .....	48
Table 41: AWGControl:RUN[:IMMediate] .....	48
Table 42: AWGControl:SREStore .....	49
Table 43: AWGControl:SSAVe .....	49
Table 44: AWGControl:STOP[:IMMediate] .....	49
Table 45: AWGControl:WAITstate.....	50
Table 46: AWGControl:JUMPMode.....	50
Table 47: AWGControl:DJStrobe .....	51
Table 48: AWGControl:DJump:FORce.....	51
Table 49: CALibration[:ALL] .....	52
Table 50: DIAGnostic[:ALL] .....	53
Table 51: OUTPut[n]:BLOffset.....	54
Table 52: OUTPut[n]:DElay .....	54
Table 53: OUTPut[n]:POLarity .....	55
Table 54: OUTPut[n]:SCALe .....	56
Table 55: OUTPut[n]:SERIESIMPedance .....	56
Table 56: OUTPut[n][:STATE] .....	57
Table 57: DIGItals:LEVel[m] .....	57
Table 58: DIGItals:NUMber .....	58
Table 59: DIGItals:SKEW[m] .....	58
Table 60: DIGItals:STATE.....	59
Table 61: DISPlay:FOCus.....	60
Table 62: DISPlay:UNIT:VOLT .....	61
Table 63: DISPlay[:WINDOW]:TEXT:CLEar.....	61
Table 64: DISPlay[:WINDOW]:TEXT[:DATA] .....	61
Table 65: HCOPY:SDUMP[:IMMediate] .....	62
Table 66: LICense:ERRor? .....	63
Table 67: LICense:HID? .....	63
Table 68: LICense: INSTall .....	64
Table 69: LICense:LIST? .....	64
Table 70: *OPT .....	64
Table 71: MARKer:LEVel[m] .....	65
Table 72: MARKer:MODE[m] .....	66
Table 73: MARKer:SKEW[m] .....	67
Table 74: ROScillator .....	68

Table 75: AWGControl:SRATE	68
Table 76: ROSCillator:SOURce	69
Table 77: *CAL	70
Table 78: *CLS	70
Table 79: *ESE	71
Table 80: *ESR	71
Table 81: *IDN?	72
Table 82: *OPC	72
Table 83: *RST	72
Table 84: *SRE	73
Table 85: *TRG	73
Table 86: *TST?	74
Table 87: *WAI	74
Table 88: PW:CREATE	75
Table 89: PW:DELETE	76
Table 90: PW:DUPLICATE	76
Table 91: PW:RENAME	77
Table 92: PW:TYPe	77
Table 93: PW:[COMmon:]CYCles	78
Table 94: PW:[COMmon:]PHAse	79
Table 95: PW:[COMmon:]FREquency	79
Table 96: PW:[COMmon:]PERiod	80
Table 97: PW:[COMmon:]LENgth	81
Table 98: PW:[COMmon:]DURation	82
Table 99: PW:[COMmon:]SRate	83
Table 100: PW:[COMmon:]ACOption	83
Table 101: PW:[COMmon:]WRAPAround	84
Table 102: PW:PULse:FALltime	85
Table 103: PW:PULse:RISetime	85
Table 104: PW:PULse:DUTycycle	86
Table 105: PW:PULse:PWIdth	87
Table 106: PW:PULse:PDElay	88
Table 107: PW:SWEep:STARtfreq	88
Table 108: PW:SWEep:STOPfreq	89
Table 109: PW:SWEep:MODE	90
Table 110: PW:SINC:PEAKpos	90
Table 111: PW:SINC:LOBewidth	91
Table 112: PW:EXP:TIMEconst	92
Table 113: PW:EXP:MODE	92

Table 114: PW:PRBs:TYPE	93
Table 115: PW:SQUare:FALLtime	94
Table 116: PW:SQUare:RISetime	94
Table 117: PW:SQUare:PDElay	95
Table 118: PW:MULTit:ADD	96
Table 119: PW:MULTit:DElete	96
Table 120: PW:MULTit:TONE[k]:FREquency?	97
Table 121: PW:MULTit:TONE[k]:AMPlitude	98
Table 122: PW:MULTit:TONE[k]:PHAsE	99
Table 123: PW:MULTit:NUM?	99
Table 124: *RCL	100
Table 125: *SAV	101
Table 126: MEMORY:NStates	101
Table 127: MEMORY:STATe:CATalog	101
Table 128: MEMORY:STATe:DElete	102
Table 129: MEMORY:STATe:LOCK	102
Table 130: MEMORY:STATe:NAME	103
Table 131: MEMORY:STATe:VALid?	104
Table 132: DElete:SETUp	104
Table 133: RECALL:SETUp	104
Table 134: MMEMory:CATalog?	105
Table 135: MMEMory:CDIRectory	106
Table 136: MMEMory:COPY	107
Table 137: MMEMory:DATA	108
Table 138: MMEMory:DATA:SIZE?	109
Table 139: MMEMory:DElete	109
Table 140: MMEMory:DOWnload:DATA	110
Table 141: MMEMory:DOWnload:FNAMe	110
Table 142: MMEMory:EXPort	111
Table 143: MMEMory:IMPort	112
Table 144: MMEMory:LOAD:ALL	114
Table 145: MMEMory:LOAD:STATe	115
Table 146: MMEMory:LOAD:STATe	115
Table 147: MMEMory:LOAD:STATe	116
Table 148: MMEMory:MSIS	116
Table 149: MMEMory:OPEN	117
Table 150: MMEMory:OPEN:SETup	118
Table 151: MMEMory:RDIRECTory	118
Table 152: MMEMory:STORe:ALL	119

Table 153: MMEMory:SAVE:SETUp .....	120
Table 154: MMEMory:STORe:STATe .....	120
Table 155: MMEMory:UPLoad? .....	121
Table 156: STATus:OPERation:CONDition? .....	122
Table 157: STATus:OPERation:ENABLE .....	122
Table 158: STATus:OPERation[:EVENT]? .....	123
Table 159: STATus:PRESet .....	123
Table 160: STATus:QUESTIONable:CONDition? .....	123
Table 161: STATus:QUESTIONable:ENABLE .....	124
Table 162: STATus:QUESTIONable[:EVENT]? .....	124
Table 163: *STB? .....	124
Table 164: *PSC .....	125
Table 165: SYSTem:BEEPer:STATE .....	126
Table 166: SYSTem:BEEPer[:IMMEDIATE] .....	126
Table 167: SYSTem:DATE .....	127
Table 168: SYSTem:ERRor[:NEXT]? .....	127
Table 169: SYSTem:KLOCK[:STATe] .....	128
Table 170: SYSTem:SECurity:IMMEDIATE .....	128
Table 171: SYSTem:TIME .....	128
Table 172: SYSTem:VERSion .....	129
Table 173: ABORT .....	130
Table 174: TRIGger[:SEQUence]:SOURce .....	130
Table 175: TRIGger[:SEQUence]:SLOPe .....	131
Table 176: TRIGger[:SEQUence]:LEVel .....	131
Table 177: TRIGger[:SEQUence]:TImer .....	132
Table 178: TRIGger[:SEQUence]:TImer:RESETCondition .....	133
Table 179: TRIGger:IMPedance .....	133
Table 180: TRIGger[:SEQUence][:IMMEDIATE] .....	134
Table 181: TRIGger[:SEQUence]:EXTMOD:ENABLE .....	134
Table 182: TRIGger[:SEQUence]:EXTMOD:Level .....	135
Table 183: TRIGger[:SEQUence]:EXTMOD:Slope .....	135
Table 184: SEQuence:ELEM[n]:AMPLitude[m] .....	136
Table 185: SEQuence:ELEM[n]:OFFset[m] .....	137
Table 186: SEQuence:ELEM[n]:VOLTage:HIGH[m] .....	137
Table 187: SEQuence:ELEM[n]:VOLTage:LOW[m] .....	138
Table 188: SEQuence:ELEM:LENGTH .....	138
Table 189: SEQuence:ELEM[n]:LOOP:COUNT .....	139
Table 190: SEQuence:ELEM[n]:WAVEform[m] .....	140
Table 191: SEQuence:LENGTH .....	140

Table 192: SEQuence:NEW .....	141
Table 193: SEQuence:FOCus .....	141
Table 194: SEQuence:ELEM[n]:WAITEvent .....	142
Table 195: SEQuence:ELEM[n]:GOTOMode .....	142
Table 196: SEQuence:ELEM[n]:GOTOEntry .....	143
Table 197: SEQuence:ELEM[n]:JUMPTOMode .....	144
Table 198: SEQuence:ELEM[n]:JUMPEvent .....	145
Table 199: SEQuence:ELEM[n]:JUMPTOEntry .....	145
Table 200: SEQuence:ELEM[n]:PATTERNEvent .....	146
Table 201: SEQuence:ELEM[n]:PATTERN .....	147
Table 202: SEQuence:ELEM[n]:PATTERNJUMPTOMode .....	148
Table 203: SEQuence:ELEM[n]:PATTERNJUMPTOEntry .....	149
Table 204: WLIST:LIST .....	150
Table 205: WLIST:NAME .....	150
Table 206: WLIST:SIZE? .....	151
Table 207: WLIST:WAVEform:DATA .....	152
Table 208: WLIST:WAVEform:DElete .....	153
Table 209: WLIST:WAVEform:IMPort .....	154
Table 210: WLIST:WAVEform:LMAXimum? .....	154
Table 211: WLIST:WAVEform:LMINimum? .....	155
Table 212: WLIST:WAVEform:LENGth? .....	155
Table 213: WLIST:WAVEform:PREDefined? .....	155
Table 214: WLIST:WAVEform:TYPE? .....	156
Table 215:MIM:CAPTure .....	157
Table 216: MIM:ID .....	157
Table 217: MIM:CAPTured .....	158
Table 218: MIM:FORward .....	158
Table 219: MIM:NUMber .....	158
Table 220: MIM:SLAve .....	159
Table 221: MIM:RELease .....	159
Table 222: Command Errors .....	162
Table 223: Predefined Waveforms .....	162

## **RESTRICTION OF HAZARDOUS SUBSTANCES (RoHS)**

Unless otherwise specified, all the materials and processes are compliant with RoHS Directive 2011/65/EU in its entirety, inclusive of any further amendments or modifications of said Directive.

## 1. PREFACE

Scope of this document is to describe the use of SCPI commands with the HD T3AWG3K-C series when used in the True-Arb Operating Mode.

### 1.1 ABBREVIATIONS AND TERMS

Abbreviation	Description
SW	Software
UI	User Interface
API	Application Programming Interface
FG	Function Generator
AM	Amplitude Modulation
FM	Frequency Modulation
PM	Phase Modulation
PWM	Pulse Width Modulation
SCPI	Standard Commands for Programmable Instruments
AWG	Arbitrary Waveform Generator
SDK	Software Development Kit
VISA	Virtual Instrument Software Architecture

Table 1: Abbreviations and terms

## 2. REVISION HISTORY

Rev.	Document Changes	Date
1.3	<p><b>Modified</b> AWGControl:RMODE</p> <p><b>Added commands:</b></p> <ul style="list-style-type: none"> <li>AWGControl:JUMPMODE {AFTERrepetitions   IMMEDIATE}</li> <li>AWGControl:JUMPMODE {AFTERrepetitions   IMMEDIATE}</li> <li>AWGControl:JUMPMODE?</li> <li>SEQUENCE:ELEM[#:]WAITEvent {NONE   MANUAL   TIMER   EXTERNAL}</li> <li>SEQUENCE:ELEM[#:]WAITEvent?</li> <li>SEQUENCE:ELEM[#:]GOTOMODE {FIRST   PREVIOUS   NEXT   LAST   ITEM}</li> <li>SEQUENCE:ELEM[#:]GOTOMODE?</li> <li>SEQUENCE:ELEM[#:]GOTOEntry {MINimum   MAXimum   DEFault   &lt;value&gt;}</li> <li>SEQUENCE:ELEM[#:]GOTOEntry? [{MINimum   MAXimum}]</li> <li>SEQUENCE:ELEM[#:]JUMPTOMODE {FIRST   PREVIOUS   NEXT   LAST   ITEM}</li> <li>SEQUENCE:ELEM[#:]JUMPTOMODE?</li> <li>SEQUENCE:ELEM[#:]JUMPEVENT {NONE   MANUAL   TIMER   EXTERNAL}</li> <li>SEQUENCE:ELEM[#:]JUMPEVENT?</li> <li>SEQUENCE:ELEM[#:]JUMTOEntry {MINimum   MAXimum   DEFault   &lt;value&gt;}</li> <li>SEQUENCE:ELEM[#:]JUMTOEntry? [{MINimum   MAXimum}]</li> <li>SEQUENCE:ELEM[#:]PATTERN {MINimum   MAXimum   DEFault   &lt;value&gt;}</li> <li>SEQUENCE:ELEM[#:]PATTERN? [{MINimum   MAXimum}]</li> <li>SEQUENCE:ELEM[#:]PATTERNJUMPTOMODE {FIRST   PREVIOUS   NEXT   LAST   ITEM}</li> <li>SEQUENCE:ELEM[#:]PATTERNJUMPTOMODE?</li> <li>SEQUENCE:ELEM[#:]PATTERNJUMTOEntry {MINimum   MAXimum   DEFault   &lt;value&gt;}</li> <li>SEQUENCE:ELEM[#:]PATTERNJUMTOEntry? [{MINimum   MAXimum}]</li> <li>AWGControl:DJStrobe</li>   <p>MIM:CAPture MIM:RELEASE MIM:ID? MIM:SLAve? MIM:FORward? MIM:CAPTured?</p> </ul>	<p><b>Commands:</b></p> <p>May 7, 2019</p>

Programming Manual – T3AWG3K-C Series Arbitrary Waveform Generator  
True-Arb Operating Mode

	MIM:NUMber?	
1.4	<b>Errata Corrigé Manual</b> OUTPut[n]:STATe return value DIGItals:NUMber add "s" of "DIGItals"	22 April 2020
1.5	<b>Added command:</b> AWGControl:DJump:FORce, TRIGger[:SEQUence]:EXTMOD:ENABLE TRIGger[:SEQUence]:EXTMOD:Level TRIGger[:SEQUence]:EXTMOD:Slope TRIGger[:SEQUence]:TImer:RESETCondition SEQUence:ELEM[#:PATTERNEvent  <b>Modified Arguments:</b> SEQUence:ELEM[#:WAItevent SEQUence:ELEM[#:JUMPEvent  <b>Corrected:</b> 'Model' parameter returned by *IDN? query: T3AWG3352, T3AWG3252, T3AWG3354, T3AWG3254, T3AWG3358, T3AWG3258	June 30, 2021
1.5.3	Correction of syntax bugs	July 12, 2022
1.5.5	<b>Command description fixed:</b> DISPLAY[:WINDOW]:TEXT[:DATA] STATUS:OPERation:CONDition? STATUS:OPERation[:EVENT]? STATUS:OPERation:CONDition? STATUS:OPERation:ENABLE? STATUS:QUESTIONable[:EVENT]? STATUS:QUESTIONable:CONDition? STATUS:QUESTIONable:ENABLE? STATUS:PRESet	October 21, 2022
1.5.6	<b>Command fixed:</b> WLIST:WAVeform:TYPE?	October 28, 2022
2.0	<b>Added application info in *IDN? command.</b>  <b>Added parametric waveform commands:</b> PW:CREATE PW:DELETE PW:DUPLICATE PW:RENAME PW:TYPE PW:[COMMON:]CYCles PW:[COMMON:]PHAsE PW:[COMMON:]FREquency PW:[COMMON:]PERiod PW:[COMMON:]ACOption PW:[COMMON:]WRAParound	November 7, 2022

**Programming Manual – T3AWG3K-C Series Arbitrary Waveform Generator  
True-Arb Operating Mode**

PW:[COMmon:]LENgth PW:[COMmon:]DURation PW:[COMmon:]SRate PW:PULse:FALLtime PW:PULse:RISetime PW:PULse:DUTycycle PW:PULse:PWlidth PW:PULse:PDelay PW:SWeep:STARTfreq PW:SWeep:STOPfreq PW:SWeep:MODE PW:SINC:PEAkpos PW:SINC:LOBewidtH PW:EXP:TIMEconst PW:EXP:MODE PW:PRBs:TYPE PW:SQuare:FALLtime PW:SQuare:RISetime PW:SQuare:PDelay PW:MULTit:ADD PW:MULTit:DELETE PW:MULTit:TONE[#:]FREquency? PW:MULTit:TONE[#:]AMPLitude PW:MULTit:TONE[#:]PHAsE PW:MULTit:NUM?	
--	--

**Table 2: Revision History**

## 3. SYNTAX AND COMMANDS

### 3.1 COMMAND SYNTAX

#### 3.1.1 SYNTAX OVERVIEW

Control the operations and functions of the instrument through the LAN interface using commands and queries. The related topics listed below describe the syntax of these commands and queries. The topics also describe the conventions that the instrument uses to process them. See the Command Groups topic for a listing of the commands by command group or use the index to locate a specific command.

Refer to the following table for the symbols that are used.

Symbol	Meaning
< >	Defined element
::=	Is defined as
	Exclusive OR
{ }	Group; one element is required
[ ]	Optional; can be omitted
...	Previous elements can be repeated
( )	Comment

Table 3: Syntax symbols and their meanings

#### 3.1.2 COMMAND AND QUERY STRUCTURE

##### Overview

Commands consist of set commands and query commands (usually called commands and queries). Commands modify instrument settings or tell the instrument to perform a specific action. Queries cause the instrument to return data and status information.

Most commands have both a set form and a query form. The query form of the command differs from the set form by its question mark on the end.

For example, the set command OUTPut1:STATE has a query form OUTPut1:STATE?.

Not all commands have both a set and a query form. Some commands have only set and some have only query.

##### Messages

A command message is a command or query name followed by any information the instrument needs to execute the command or query. Command messages may contain five element types, defined in the following table.

Symbol	Meaning
<Header>	This is the basic command name. If the header ends with a question mark, the command is a query. The header may begin with a colon (:) character. If the command is concatenated with other commands, the beginning colon is required. Never use the beginning colon with command headers beginning with a star (*).
<Mnemonic>	This is a header subfunction. Some command headers have only one mnemonic. If a command header has multiple mnemonics, a colon (:) character always separates them from each other.
<Argument>	This is a quantity, quality, restriction, or limit associated with the header. Some commands have no arguments while others have multiple arguments. A <space> separates arguments from the header. A <comma> separates arguments from each other.
<Comma>	A single comma is used between arguments of multiple-argument commands. Optionally, there may be white space characters before and after the comma.
<Space>	A white space character is used between a command header and the related argument. Optionally, a white space may consist of multiple white space characters.

**Table 4: Message symbols and their meanings**

## Commands

Commands cause the instrument to perform a specific function or change one of the settings. Commands have the structure:

[:]<Header>[<Space><Argument>[<Comma><Argument>]...]

A command header consists of one or more mnemonics arranged in a hierarchical or tree structure. The first mnemonic is the base or root of the tree and each subsequent mnemonic is a level or branch of the previous one. Commands at a higher level in the tree may affect those at a lower level. The leading colon (:) always returns you to the base of the command tree.

## Queries

Queries cause the instrument to return status or setting information.

Queries have the structure:

[:]<Header>?

[:]<Header>?[<Space><Argument>[<Comma><Argument>]...]

### 3.1.3 COMMAND ENTRY

#### Rules

The following rules apply when entering commands:

- You can enter commands in upper or lower case.
- You can precede any command with white space characters. White space characters include any combination of the ASCII control characters 00 through 09 and 0B through 20 hexadecimal (0 through 9 and 11 through 32 decimal).
- The instrument ignores commands consisting of any combination of white space characters and line feeds.

#### Abbreviating

You can abbreviate many instrument commands. Each command in this documentation shows the abbreviations in capitals. For example, enter the command AWGControl:RMODE TRIGgered simply as AWGC:RMODE TRIG.

#### Concatenating

Use a semicolon (;) to concatenate any combination of set commands and queries.

The instrument executes concatenated commands in the order received. When concatenating commands and queries, follow these rules:

1. Separate completely different headers by a semicolon and by the beginning colon on all commands except the first one.

For example, the commands OUTPut1:STATe ON and AWGControl:RMODE TRIGgered, can be concatenated into the following single command:  
OUTPut1:STATe ON;:AWGControl:RMODE TRIGgered.

2. If concatenated commands have headers that differ by only the last mnemonic, abbreviate the second command and eliminate the beginning colon.

For example, concatenate the commands SEQuence:ELEM1:VOLTage:HIGH1 2 and SEQuence:ELEM1:VOLTage:LOW1 -2 into a single command:

SEQuence:ELEM1:VOLTage:HIGH1 2;LOW1 -2

The longer version works equally well:

SEQuence:ELEM1:VOLTage:HIGH1 2;; SEQuence:ELEM1:VOLTage:LOW1 -2

3. Never precede a star (\*) command with a semicolon (;) or colon (:).

4. When you concatenate queries, the responses to all the queries are concatenated into a single response message.

For example, if the high level of the marker1 of channel one is 1.0 V and the voltage selection is LINE, the concatenated query : MARKer:LEVel1?; : MARKer:MODE?; will return the following:

1.0;FIXEDLow

5. Set commands and queries may be concatenated in the same message.

For example, AWGControl:RMODE CONTinuous::SEQUence:LENGth? is a valid message that sets the run mode to Sequence. The message then queries the length of the sequence. Concatenated commands and queries are executed in the order received.

Here are some invalid concatenations:

- OUTPut1:STATe ON;AWGControl:RMODE CONTinuous  
(no colon before AWGControl)
- SEQuence:ELEM1:VOLTage:HIGH1 2;;LOW1 -2 (extra colon before LOW1 -2 instead  
SEQuence:ELEM1:VOLTage:HIGH1 2;LOW1 -2)

### **Terminating**

This documentation uses <EOM> (end of message) to represent a message terminator.

Symbol	Meaning
<EOM>	Message terminator

**Table 5: Message terminator and meaning**

For messages sent to the instrument, the end-of-message terminator must be the END message (EOI asserted concurrently with the last data byte). The instrument always terminates messages with LF and EOI. It allows white space before the terminator. For example, it allows CR LF.

#### 3.1.4 PARAMETER TYPES

Parameters are indicated by angle brackets, such as <file\_name>. There are several different types of parameters, as listed in the following table. The parameter type is listed after the parameter. Some parameter types are defined specifically for the instrument command set and some are defined by SCPI.

Parameter type	Description	Example
Arbitrary block	A block of data bytes	#512234xxxx... where 5 indicates that the following 5 digits (12234) specify the length of the data in bytes; xxxx... indicates actual data or #0xxxx...<LF><&EOI>
Boolean	Boolean numbers or values	ON or 1 OFF or 0
Discrete	A list of specific values	MINimum, MAXimum
NR1 numeric	Integers	0, 1, 15, -1
NR2 numeric	Decimal numbers	1.2, 3.141, -6.5

NR3 numeric	Floating point numbers	3.1415E+9
NRf numeric	Flexible decimal numbers that may be type NR1, NR2, or NR3	See NR1, NR2, and NR3 examples in this table
String	Alphanumeric characters (must be within quotation marks)	"Testing 1, 2, 3"

**Table 6: Parameter types, their descriptions, and examples**

### Quoted String

Some commands accept or return data in the form of a quoted string, which is simply a group of ASCII characters enclosed by a single quote ('') or double quote (""). For example: "this is a quoted string". This documentation represents these arguments as follows:

Symbol	Meaning
<QString >	Quoted string of ASCII text

**Table 7: String symbol and meaning**

A quoted string can include any character defined in the 7-bit ASCII character set. Follow these rules when you use quoted strings:

1. Use the same type of quote character to open and close the string. For example: "this is a valid string".
2. You can mix quotation marks within a string as long as you follow the previous rule. For example, "this is an 'acceptable' string".
3. You can include a quote character within a string simply by repeating the quote. For example: "here is a "" mark".
4. Strings can have upper or lower case characters.
5. A carriage return or line feed embedded in a quoted string does not terminate the string, but is treated as just another character in the string.
6. The maximum length of a quoted string returned from a query is 1000 characters.

Here are some invalid strings:

- "Invalid string argument" (quotes are not of the same type)
- "test<EOI>" (termination character is embedded in the string)

### Units and SI Prefix

If the decimal numeric argument refers to voltage, frequency, impedance, or time, express it using SI units instead of using the scaled explicit point input value format <NR3>. (SI units are units that conform to the System International d'Unites standard.) For example, use the input format 200 mV or 1.0 MHz instead of 200.0E-3 or 1.0E+6, respectively, to specify voltage or frequency.

Omit the unit when you describe commands, but include the SI unit prefix. Enter both uppercase and lowercase characters. The following list shows examples of units you can use with the commands.

- V for voltage (V).
- HZ for frequency (Hz).
- OHM for impedance (ohm).
- S for time (s).
- DBM for power ratio.
- PCT for %.
- VPP for Peak-to-Peak Voltage (V p-p).
- UIPP for Peak-to-Peak, Unit is UI (UI p-p).
- UIRMS for RMS, Unit is UI (Ulrms).
- SPP for Peak-to-Peak, Unit is second (s p-p).
- SRMS for RMS, Unit is second (srms).
- V/NS for SLEW's unit (V/ns).

In the case of angles, use RADian and DEGree. The default unit is RADian. The SI prefixes, which must be included, are shown in the following table. You can enter both uppercase and lowercase characters.

SI prefix <sup>1</sup>	Corresponding power
EX	$10^{18}$
PE	$10^{15}$
T	$10^{12}$
G	$10^9$
MA	$10^6$
K	$10^3$
M	$10^{-3}$
U <sup>2</sup>	$10^{-6}$
N	$10^{-9}$
P	$10^{-12}$
F	$10^{-15}$
A	$10^{-18}$

**Table 8: SI prefixes and their indexes**

1. Note that the prefix m/M indicates  $10^{-3}$  when the decimal numeric argument denotes voltage or time, but indicates  $10^6$  when it denotes frequency.
2. Note that the prefix u/U is used instead of “ $\mu$ ”.


Since M (m) can be interpreted as 1E-3 or 1E6 depending on the units, use mV for V, and MHz for Hz.

The SI prefixes need units.  
Correct: 10MHz, 10E+6Hz, 10E+6  
Incorrect: 10M

### 3.1.5 SCPI COMMANDS AND QUERIES

The arbitrary waveform generator uses a command language based on the SCPI standard. The SCPI (Standard Commands for Programmable Instruments) standard was created by a consortium to provide guidelines for remote programming of instruments. These guidelines provide a consistent programming environment for instrument control and data transfer. This environment uses defined programming messages, instrument responses and data formats that operate across all SCPI instruments, regardless of manufacturer.

The SCPI language is based on a hierarchical or tree structure that represents a subsystem (see following figure). The top level of the tree is the root node; it is followed by one or more lower-level nodes.

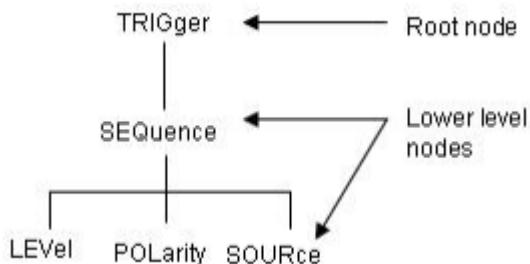

You can create commands and queries from these subsystem hierarchy trees. Commands specify actions for the instrument to perform. Queries return measurement data and information about parameter settings.

## 4. The Registers

### 4.1 STATUS AND EVENTS


The SCPI interface in the instrument includes a status and event reporting system that enables the user to monitor crucial events that occur in the instrument.

#### 4.1.1 STATUS AND EVENT REPORTING SYSTEM

The following figure outlines the status and event reporting mechanism offered in the arbitrary waveform generators. It contains three major blocks:

- Standard Event Status
- Operation Status
- Questionable Status (fan-out structure, not used in this version).

The processes performed in these blocks are summarized in the Status Byte.

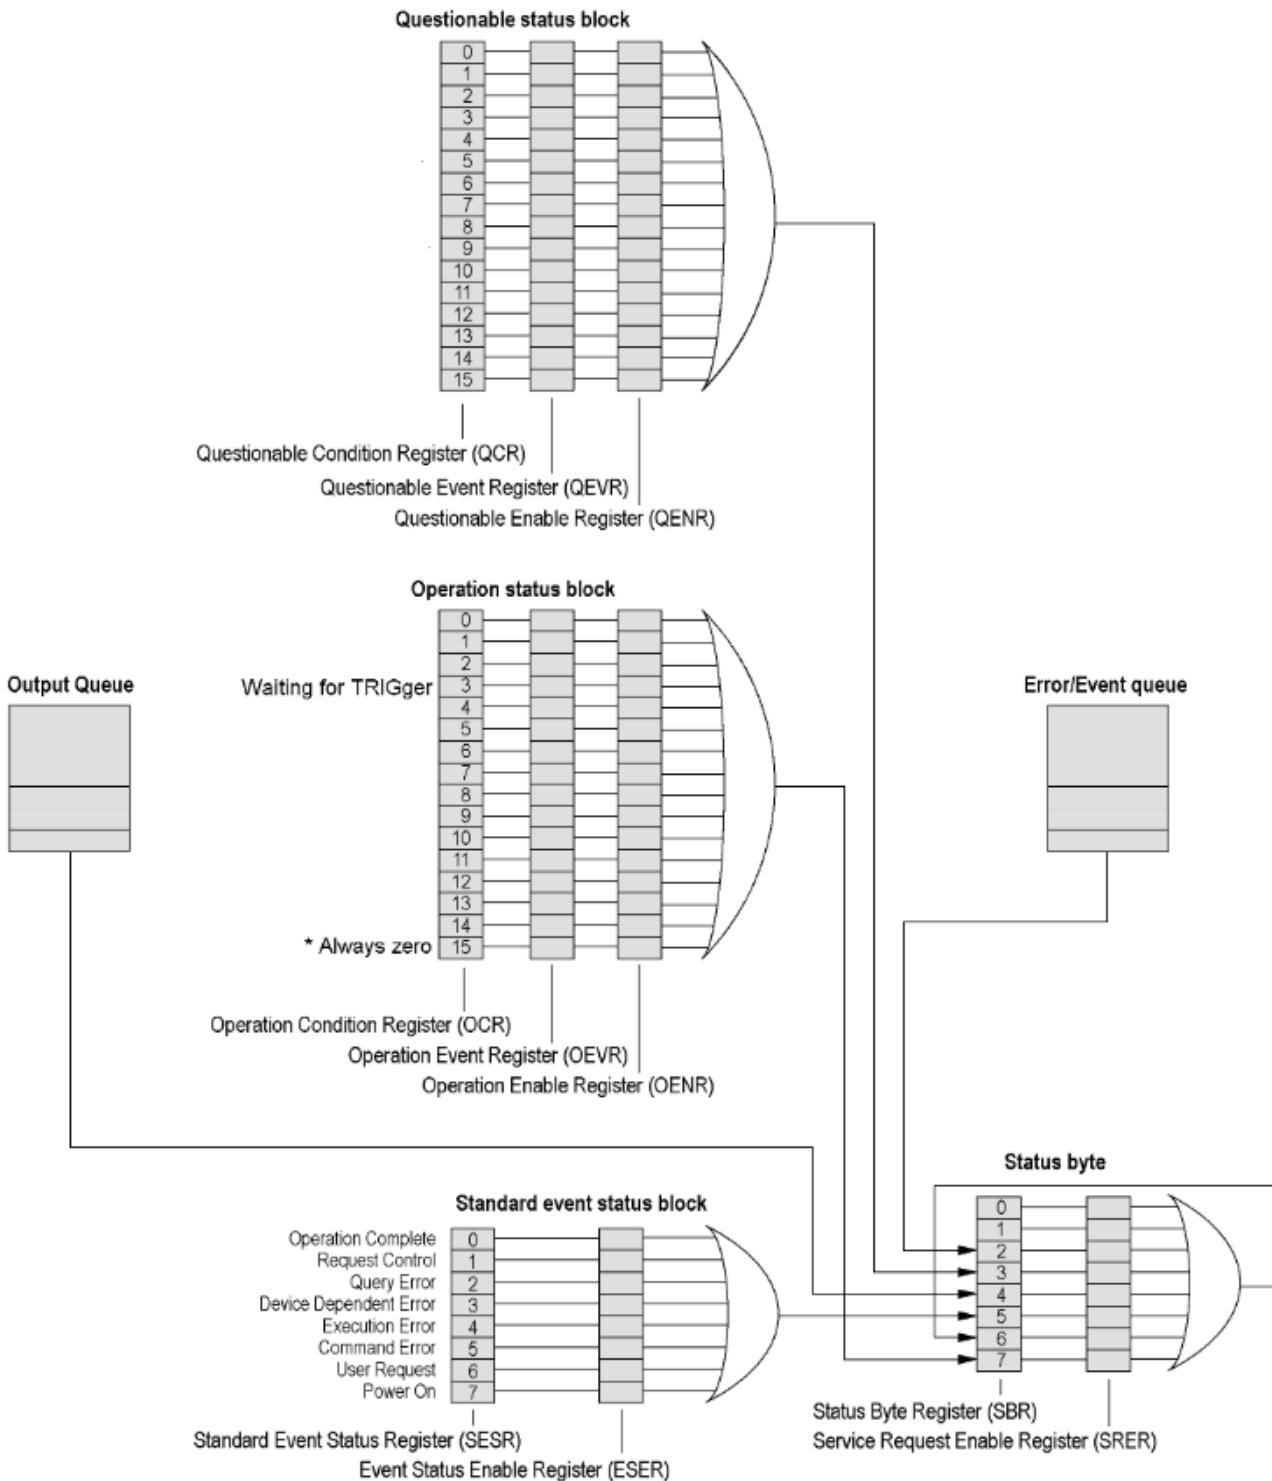

#### 4.1.2 STATUS BYTE REGISTER (SBR)

The bits of this register are used to monitor the output queue, SESR and service requests, respectively. The contents of this register are returned when the \*STB? query is used.

<b>BIT</b>	<b>Name</b>	<b>Description</b>
7 (MSB)	OSS	Operation Summary Status (OSS). Summary of the operation status register.
6	RQS/MSS	Request Service (RQS)/Master Status Summary (MSS). When the instrument is accessed using the serial poll command, this bit is called the Request Service(RQS) bit and indicates to the controller that a service request has occurred. The RQS bit is cleared when serial poll ends. When the instrument is accessed using the *STB? query, this bit is called the Master Status Summary (MSS) bit and indicates that the instrument has issued a service request for one or more reasons. The MSS bit is never cleared to 0 by the *STB? Query.
5	ESB	Event Status Bit (ESB). This bit indicates whether or not a new event has occurred after the previous Standard Event Status Register (SESR) has been cleared or after an event readout has been performed
4	MAV	Message Available Bit (MAV). This bit indicates that a message has been placed in the output queue and can be retrieved.
3	QSS	Questionable Summary Status (QSS). Summary of the Questionable Status Byte register.
2	EAV	Event Quantity Available (EAV). Summary of the Error Event Queue.
1	--	This is not used
0(LSB)	--	This is not used

**Table 9: Status Byte Register (SBR)**

#### 4.1.3 SERVICE REQUEST ENABLE REGISTER (SRER)

The SRER is made up of bits defined exactly the same as bits 0 through 7 in the SBR as shown in the following figure. This register is used by the user to determine what events will generate service requests.

The SRER bit 6 cannot be set. Also, the RQS is not maskable.

The generation of a service request with the GPIB interface involves changing the SRQ line to LOW and making a service request to the controller. The result is that a status byte for which an RQS has been set is returned in response to serial polling by the controller.

Use the \*SRE command to set the bits of the SRER. Use the \*SRE? query to read the contents of the SRER. Bit 6 must normally be set to 0.

7	6	5	4	3	2	1	0
OSB	--	ESB	MAV	QSB	--	--	--

**Table 10: Service Request Enable Register (SRER)**

#### 4.1.4 STANDARD EVENT STATUS BLOCK (SESB)

Reports the power on/off state, command errors, and the running state. It consists of the following registers:

- Standard Event Status Register (SESR)
- Event Status Enable Register (ESER)

These registers are made up of the same bits defined in the following table. Use the \*ESR? query to read the contents of the SESR. Use the \*ESE() command to access the ESER

##### 4.1.4.1 Standard Event Status Register (SESR)

BIT	Name	Description
7 (MSB)	PON	Power On (PON). Indicates that the power to the instrument is on.
6	--	Not used.
5	CME	Command Error (CME). Indicates that a command error has occurred while parsing by the command parser was in progress.

<b>BIT</b>	<b>Name</b>	<b>Description</b>
4	EXE	Execution Error (EXE). Indicates that an error occurred during the execution of a command. Execution errors occur for one of the following reasons: <ul style="list-style-type: none"> <li>• when a value designated in the argument is outside the allowable range of the instrument, or is in conflict with the capabilities of the instrument.</li> <li>• when the command could not be executed properly because the conditions for execution differed from those essentially required.</li> </ul>
3	DDE	Device-Dependent Error (DDE). An instrument error has been detected.
2	QYE	Query Error (QYE). Indicates that a query error has been detected by the output queue controller. Query errors occur for one of the following reasons: <ul style="list-style-type: none"> <li>• an attempt was made to retrieve messages from the output queue, despite the fact that the output queue is empty or in pending status.</li> <li>• the output queue messages have been cleared despite the fact that they have not been retrieved.</li> </ul>
1	--	Not used.
0 (LSB)	OPC	Operation Complete (OPC). This bit is set with the results of the execution of the *OPC command. It indicates that all pending operations have been completed.

**Table 11: Standard Event Status Register (SESR)**

When an event occurs, the SESR bit corresponding to the event is set, resulting in the event being stacked in the Error/Event Queue. The SBR OAV bit is also set. If the bit corresponding to the event has also been set in the ESR, the SBR ESB bit is also set. When a message is sent to the Output Queue, the SBR MAV bit is set.

#### 4.1.5 OPERATION STATUS BLOCK

The operation status block contains conditions that are part of the instrument's normal operation. It consists of the following registers:

- Operation Condition Register (OCR)

- Operation Event Register (OEVR)
- Operation Enable Register (OENR)

These registers are made up of the same bits defined in the following table. Use the STA-Tus:OPERation commands to access the operation status register set.

#### 4.1.5.1 Operation Condition Register (OCR)

15	14	13	12	11	10	9	8	7	6	5	4	3	2	1	0
--	--	--	--	--	--	--	--	--	--	--	--	WFT	--	--	--

**Table 12: Operation Condition Register (OCR)**

Bit3 Waiting for trigger (WFT): indicates that the instrument is waiting for a trigger event to occur.

When the specified state changes in the OCR, its bit is set or reset. This change is filtered with a transition register, and the corresponding bit of the OEVR is set.

If the bit corresponding to the event has also been set in the OENR, the SBR OSS bit is also set.

#### 4.1.6 QUESTIONABLE STATUS BLOCK

The questionable status register set contains bits which give an indication of the quality of various aspects of the signal together with the fanned out registers as described in the next subsections. It consists of the following registers:

- Questionable Condition Register (QCR)
- Questionable Event Register (QEVR)
- Questionable Enable Register (QENR)

Despite the commands to query these registers are usable (see STATus:QUESTIONable commands) , these register are not used in this version.

## 4.2 ANALOG DATA FORMAT (.TXT FILE ONLY)

The analog waveform can be imported into the instrument using a .txt file. For analog waveform you have to create a single column of values (signed integer or signed decimal, the header is not allowed) separated with 'new line'. These values are imported into the instrument normalized so that the user can easily adjust waveform's amplitude/offset using the corresponding SCPI commands (see SEQuence:ELEM[n]:AMPlitude[m], SEQuence:ELEM[n]:OFFset[m] or SEQuence:ELEM[n]:VOLTage:HIGH[m], SEQuence:ELEM[n]:VOLTage:LOW[m] commands).

## 4.3 DIGITAL DATA FORMAT (.TXT FILE ONLY)

For digital waveform you have to create a single column of values (unsigned integer range [0..(2<sup>32</sup> - 1)], the header is not allowed) separated with 'new line'. In this way each value converted into 32-bits binary format represents the status of the corresponding digital line (Bit 0 -> Digital Line 0, Bit 1 -> Digital Line 1, ..., Bit 31 -> Digital Line 31).

For example the integer value 5789 matches the binary value 00000000000000000000001011010011101, thereby the status of digital Pads is:

Digital Pod A

1	0	0	1	1	1	0	1
Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0

Digital Pod B

0	0	0	1	0	1	1	0
Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0

Digital Pod C

0	0	0	0	0	0	0	0
Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0

Digital Pod D

0	0	0	0	0	0	0	0
Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0

If the configuration of the instrument implies that some pods are not present or enabled the corresponding bits are meaningless.

The digital outputs sampling rate is the same of the analog sampling rate, so the length of the digital samples must be the same of the analog waveform length.

Example: analog waveform length = 100 samples

→ digital waveform length = 100 samples

#### 4.4 GRANULARITY

The minimum waveform length is 16 samples.

From 16 to 384 samples the granularity is 16.

With waveform's length greater than 384 the granularity is 1.

#### 4.5 TRANSFERRING DATA FILE

When transferring data file, it is convenient to send data in chunks. This allows better memory management and enables you to stop the transfer before it is completed. It also helps the external controller to report the progress of the operation to the user.

##### 4.5.1 BLOCK DATA FORMAT

Block data is a transmission format which is suitable for the transmission of large amounts of data. A command using a block data parameter with definite length has the following structure:

**Example:** HEADER:HEADER #45168xxxxxxxx

The hash symbol # introduces the data block. The next number indicates how many of the following digits describe the length of the data block. In the example the 4 following digits indicate the length to be 5168 bytes. The data bytes follow. During the transmission of these data bytes all End or other control signs are ignored until all bytes are transmitted.

#### 4.6 BYTE ORDER DURING TRANSFER

Waveform data is always transferred using little-endian format.

#### 4.7 HOW TO GENERATE AN ARBITRARY WAVEFORM

If you need to generate an arbitrary waveform and reproduce it on your instrument, you can follow the instructions below:

1. Generate a .txt file with the waveform samples; fill the .txt file with all arbitrary samples paying attention to data format (see analog/digital data format chapters for more details).
2. Transfer the .txt file from client PC to mass storage memory of the instrument (see MMEMory:DATA command and Block Data Format chapter for more details about this operation).
3. Import the .txt file in waveform list (see WLIST:WAveform:IMPort command which also allows you to choose an appropriate name for the new imported waveform, i.e. "Wave\_name").
4. Insert "Wave\_name" waveform in the first entry of sequencer and on the desired channel (see SEQuence:ELEM[n]:WAveform[m] command).
5. Set the desired running mode (AWGControl:RMODE) and output parameters.
6. Enable the outputs (OUTPut[n][:STATe] or DIGItals:STATe).
7. Send a start command (AWGControl:RUN).

## 5. COMMAND GROUPS

The following commands refer to the parameters [n] and [m] that depend on the instrument model.

Instrument Model	Parameter [n] = Available Channels	Parameter [m] = Available Outputs
T3AWG3252, T3AWG3352	1 2	1
T3AWG3254, T3AWG3354	1 2 3 4	1 2
T3AWG3258, T3AWG3358	1 2 3 4 5 6 7 8	1 2 3 4

Table 13: Models and available parameters

### 5.1 CONTROL GROUP COMMANDS

Use the following commands to control operating modes:

Command	Description
AWGControl:AFGSwitch	Turns off the TrueArb application and runs the Simple AFG application
AWGControl:BURST	Sets or returns the Burst Count parameter
AWGControl:CONFigure:CNUMber?	Returns the number of analog channels available on the instrument
AWGControl:CONFigure:DNUMber?	Returns the number of digital channels available on the AWG
AWGControl:DECreasing	Sets or returns the Sample Dcreasing Strategy parameter
AWGControl:INCreasing	Sets or returns the Sample Increasing Strategy parameter
AWGControl:LENGTH:MODE	Sets or returns the Entry Length Strategy parameter
AWGControl:RESET[:IMMEDIATE]	This command resets sequence to its default state.
AWGControl:RMODE	This command sets or returns the AWG run mode.
AWGControl:RSTATE?	Returns the state of the arbitrary waveform generator.
AWGControl:RUN[:IMMEDIATE]	Initiates the output of a waveform or a sequence

Command	Description
AWGControl:SREStore	Opens a setup file into the AWG's setup memory
AWGControl:SSAVe	Saves the AWG's setup with waveforms
AWGControl:STOP[:IMMEDIATE]	Stops the output of a Sequence
AWGControl:WAITstate	Sets or returns the Wait Trigger On parameter
AWGControl:JUMPMODE	Sets or returns the Jump Mode parameters
AWGControl:DJStrobe	Sends the pattern strobe event
AWGControl:DJump:FORce	Allows to jump to the specified entry of the sequencer.

**Table 14: Control group commands**

## 5.2 CALIBRATION AND DIAGNOSTIC COMMANDS

Command	Description
CALibration[:ALL]	Performs a full calibration of the AWG. The query form performs a full calibration and returns a status of the operation.
DIAGnostic[:ALL]	Performs the self diagnostic procedure.

**Table 15: Calibration and Diagnostic group commands**

## 5.3 OUTPUT GROUP COMMANDS

Use the following output commands to set or return the characteristics of the output port of the arbitrary waveform generator:

Command	Description
OUTPut[n]:BLOffset	Sets or returns the Base Line Offset parameter of the channel n.
OUTPut[n]:DELay	Sets or returns the Skew parameter of the analog channel "n".
OUTPut[n]:POLarity	Sets or returns the Polarity parameter of the channel n

OUTPut[n]:SCALe	Sets or returns the Amplitude Scale parameter of the channel n
OUTPut[n]:SERIESIMPedance	Sets or returns the Output Impedance parameter for the channel n.
OUTPut[n][:STATe]	Sets or returns the channel n state.
DIGItals:LEVel[m]	Sets or returns the Voltage Level of the selected Digital Probe "m"
DIGItals:NUMber	Sets or returns the number of the Digital Channels.
DIGItals:SKEW[m]	Sets or returns the Skew parameter for the selected Digital Probe "m"
DIGItals:STATe	Sets or returns the state of the digital channels.

**Table 16: Output group commands**

## 5.4 DISPLAY COMMANDS

Display commands let you to manage features related to the user interface.

Command	Description
DISPlay:FOCuS	Selects the channel displayed "in front" on the AWG
DISPlay:UNIT:VOLT	Selects the method for specifying voltage ranges
DISPlay[:WINDOW]:TEXT:CLEar	Delete text message
DISPlay[:WINDOW]:TEXT[:DATA]	Set or query the text message display
HCOPy:SDUMP[:IMMEDIATE]	Copy screen image and save it in the specified file.

**Table 17: Display group commands**

## 5.5 LICENSE COMMANDS

License commands let you to manage features related to the options that can be installed through a license file.

Command	Description
LICense:ERRor?	This query-only command returns a code about license options loading operation.

Command	Description
LICense:HID?	Returns the instrument HostID unique identifier.
LICense:INSTall	Accepts a license and installs it on the instrument.
LICense:LIST?	Returns the license codes as a comma-separated list of string.
*OPT?	Returns the implemented options for the AWG.

**Table 18: License group commands**

## 5.6 MARKER COMMANDS

Use the following marker commands to set and query the marker output parameter:

Command	Description
MARKer:LEVel[m]	Sets or returns the Voltage Level parameter of the Marker “m”
MARKer:MODE[m]	Sets or returns the Marker Mode parameter of the Marker “m”
MARKer:SKEW[m]	Sets or returns the Marker Skew parameter of the Marker “m”

**Table 19: Marker group commands**

## 5.7 CLOCK GROUP COMMANDS

Use the following commands to set and query the reference and sampling clock parameters

Command	Description
ROSCillator	Sets or returns the reference clock value in Hz
ROSCillator:SOURce	Sets or returns the reference clock source to internal or external
AWGControl:SRATE	This command sets or returns the sample rate for the clock

**Table 20: Clock group commands**

## 5.8 IEEE MANDATED AND OPTIONAL GROUP COMMANDS

All AWG IEEE mandated and optional command implementations are based on the SCPI standard and the specifications for devices in IEEE 488.2.

Command	Description
*CAL?	Runs the self calibration and returns the result. Same as CALibration[:ALL].
*CLS	Clears all event registers and queues.
*ESE	This command sets or returns the status of Event Status Enable Register (ESER). (See Status and events chapter).
*IDN?	This command returns identification information for the AWG. Refer to Std IEEE 488.2 for additional information.
*OPC	This command causes the AWG to sense the internal flag referred to as the “No-Operation-Pending” flag. The command sets bit 0 in the Standard Event Status Register when pending operations are complete. The query form returns a “1” when the last overlapping command operation is finished.
*RST	Resets the AWG to its default state.
*SRE	Sets or returns the bits in the Service Request Enable Register (SRER).
*TRG	This command generates a trigger event. This is equivalent to press and release the trigger button on the front panel.
*TST?	Executes the Self Diagnostic Procedure and returns the result.
*WAI	Ensures the completion of the previous command before the next command is issued.

**Table 21: IEEE Mandatory group commands**

## 5.9 PARAMETRIC WAVEFORMS COMMANDS

Use the following commands to set and query the parametric waveforms parameters.

Command	Description
PW:CREATE	This command creates a new parametric waveform
PW:DELETE	Deletes a parametric waveform

<b>Command</b>	<b>Description</b>
PW:DUPLICATE	Creates a copy of a parametric waveform
PW:RENAME	Rename a specified waveform (parametric, predefined or not predefined)
PW:TYPE	Sets or queries the type of the parametric waveform
PW:[COMMON:]CYCles	Sets or queries the cycles parameter of a parametric waveform
PW:[COMMON:]PHAsE	Sets or queries the phase parameter of a parametric waveform
PW:[COMMON:]FREquency	Sets or queries the frequency parameter of a parametric waveform
PW:[COMMON:]PERiod	Sets or queries the period parameter of a parametric waveform
PW:[COMMON:]LENgth	Sets or queries the length parameter of a parametric waveform
PW:[COMMON:]DURation	Sets or queries the duration parameter of a parametric waveform
PW:[COMMON:]SRate	Sets or queries the sampling rate parameter of a parametric waveform
PW:[COMMON:]ACOption	Sets or returns the strategy of Auto Calc Option
PW:[COMMON:]WRAPAround	Sets or queries the status of Wrap Around parameter
PW:PULse:FALltime	Sets or queries the fall time of a parametric pulse waveform
PW:PULse:RISetime	Sets or queries the rise time of a parametric pulse waveform
PW:PULse:DUTycycle	Sets or queries the duty cycle of a parametric pulse waveform
PW:PULse:PWldth	Sets or queries the pulse width of a parametric pulse waveform
PW:PULse:PDElay	Sets or queries the pulse delay of a parametric pulse waveform
PW:SWEep:STArtfreq	Sets or queries the start frequency parameter of a parametric sweep waveform
PW:SWEep:STOPfreq	Sets or queries the stop frequency parameter of a parametric sweep waveform
PW:SWEep:MODE	Sets or queries the sweep mode parameter of a parametric sweep waveform

<b>Command</b>	<b>Description</b>
PW:SINC:PEAkpos	Sets or queries the peak position of a parametric sinc waveform
PW:SINC:LOBewith	Sets or queries the lobe width of a parametric sinc waveform
PW:EXP:TIMEconst	Sets or queries the time constant of a parametric exponential waveform
PW:EXP:MODE	Sets or queries the mode of a parametric exponential waveform
PW:PRBs:TYPE	Sets or queries the Prbs order of a parametric Prbs waveform
PW:SQUare:FALLtime	Sets or queries the fall time of a parametric square waveform
PW:SQUare:RISetime	Sets or queries the rise time of a parametric square waveform
PW:SQUare:PDElay	Sets or queries the pulse delay of a parametric square waveform
PW:MULTit:ADD	Creates a new sinusoidal tone in a parametric multitone waveform
PW:MULTit:DELETE	Deletes all or a single tone in a parametric multitone waveform
PW:MULTit:TONE[k]:FREQUENCY?	Returns the frequency of a tone of a parametric multitone waveform
PW:MULTit:TONE[k]:AMPLITUDE	Sets or queries the amplitude of a parametric multitone waveform
PW:MULTit:TONE[k]:PHASE	Sets or queries the phase of a parametric multitone waveform
PW:MULTit:NUM?	Returns the total number of tones of a parametric multitone waveform

**Table 22: Parametric Waveforms Commands**

## 5.10 STATUS GROUP COMMANDS

The external controller uses the status commands to coordinate operation between the TrueArb and other devices on the bus. The status commands set and query the registers/queues of the TrueArb event/status reporting system. For more information about registers and queues, see Status and Event reporting section.

<b>Command</b>	<b>Description</b>
*CLS	Clears all event registers and queues
*ESE	Sets or queries the status of Event Status Enable Register (ESER)
*ESR?	Returns the status of Standard Event Status Register (SESR)
*SRE	Sets or queries the bits in Service Request Enable Register (SRER)
STATus:OPERation:CONDition?	Returns the contents of the Operation Condition Register (OCR)
STATus:OPERation:ENABLE	Sets or returns the mask for the Operation Enable Register (OENR)
STATus:OPERation[:EVENT]?	Returns the contents of Operation Event Register (OEVR)
STATus:PRESet	Sets the OENR and QENR registers.
STATus:QUESTIONable:CONDition?	Returns the status of the Questionable Condition Register (QCR)
STATus:QUESTIONable:ENABLE	Sets or returns the mask for Questionable Enable Register (QENR).
STATus:QUESTIONable[:EVENT]?	Returns the status of the Questionable Event (QEVR) Register and clears it– Not used.
*STB?	Returns the contents of Status Byte Register (SBR).
*PSC	Set or query power-on status clear

**Table 23:Status group commands**

## 5.11 SYSTEM GROUP COMMANDS

Use the following system commands to control miscellaneous instrument functions:

<b>Command</b>	<b>Description</b>
SYSTem:BEEPer:STATE	Sets or queries the beeper state
SYSTem:BEEPer[:IMMEDIATE]	Generates an audible tone
SYSTem:DATE	Sets or returns the system date.
SYSTem:ERRor[:NEXT]?	Returns data from the error and event queue.
SYSTem:KLOCK[:STATE]	Sets or queries the front panel lock/unlock
SYSTem:SECurity:IMMEDIATE	Resets to factory default
SYSTem:TIME	Sets or returns the system time.

SYSTem:VERSION?	Returns the SCPI version number to which the command conforms.
-----------------	--

**Table 24: System group commands**

## 5.12 MEMORY GROUP COMMANDS

Memory commands let you manage the setup memory. The following table describes the memory commands.

Command	Description
*RCL	Recall instrument settings from setup memory
*SAV	Save instrument settings to setup memory
MEMory:NStates?	Returns the total number of available configurations saved in the AWG.
MEMory:STATe:CATalog?	List the names of available configurations saved in the AWG.
MEMory:STATe:DElete	Delete a configuration saved in the AWG.
MEMory:STATe:DElete	Delete the setup memory
MEMory:STATe:LOCK	Sets or queries the lock of configuration overwrite and deletion
MEMory:STATe:NAME	Copies a configuration.
MEMory:STATe:VALid?	Queries the availability of a configuration.
DElete:SETUp	Deletes a configuration.
RECALL:SETUp	Restores the instrument settings from a configuration name.

**Table 25: Memory Group commands**

## 5.13 MASS MEMORY COMMANDS

Mass memory commands let you change mass memory attributes. The following table describes the mass memory commands.

Command	Description
MMEMemory:CATalog?	Returns the entire list of files and directory located in the current directory.
MMEMemory:CDIRectory	Sets or returns the current directory of the file system on the AWG.
MMEMemory:COPY	Copies a source file in a target file.

<b>Command</b>	<b>Description</b>
MMEMory:DATA	Sets or returns block data to/from file in the current mass storage device.
MMEMory:DATA:SIZE?	Returns the size in bytes of a selected file.
MMEMory:DElete	Deletes a file or directory from the AWG's files system.
MMEMory:DOWNload:DATA	Downloads data from the host computer to instrument's Mass Memory.
MMEMory:DOWNload:FNAME	Specifies file name for downloading data from the computer to instrument's Mass Memory.
MMEMory:EXPort	Exports a waveform from the current waveform list to an archive file (.zip).
MMEMory:IMPort	Imports a file into the AWG's waveform list.
MMEMory:LOAD:ALL	Loads an AWG's configuration file and set it as current configuration.
MMEMory:LOAD:STATe	Loads an AWG's configuration file in the configurations list.
MMEMory:MDIRectory	Creates a new directory in the current path on the Mass Memory system.
MMEMory:MOVE	Moves a file on Mass Memory device.
MMEMory:MSIS	Sets or returns a mass storage device used by all MMEMory commands.
MMEMory:OPEN	Loads a file into the AWG waveform list.
MMEMory:OPEN:SETup	Loads an AWG's configuration file and set it as current configuration.
MMEMory:RDIRectory	Removes an empty directory.
MMEMory:SAVE:SETup	Saves the current configuration in an archive (.zip).
MMEMory:STORe:ALL	Saves the current configuration in an archive (.zip).
MMEMory:STORe:STATe	Saves a configuration present in the configurations list in an archive (.zip)
MMEMory:UPLoad?	Returns the contents of a file.

**Table 26: Mass Memory Group commands**

## 5.14 TRIGGER GROUP COMMANDS

The trigger commands let you control all aspects of triggering. The following table describes the trigger input commands.

Command	Description
ABORT	Reset and initialize the trigger system
TRIGger[:SEQUence][:IMMEDIATE]	Generates a trigger event
TRIGger[:SEQUence]:SLOPe	Set or query the slope of the trigger input signal
TRIGger[:SEQUence]:SOURce	Set or query the source of the trigger input signal
TRIGger[:SEQUence]:LEVel	Set or query the trigger threshold level of an input signal
TRIGger[:SEQUence]:TImer	Set or query the internal rate of the timer
TRIGger[:SEQUence]:TImer:RESETCondition	Set or query the condition for resetting the timer
TRIGger:IMPedance	Set or query the trigger input impedance
TRIGger[:SEQUence]:EXTMOD:ENABLE	Set or query the status of Ext. Mod. signal
TRIGger[:SEQUence]:EXTMOD:Level	Set or query the threshold of Ext. Mod. input signal applied to Ext Mod In SMA connector
TRIGger[:SEQUence]:EXTMOD:Slope	Set or query the slope of Ext. Mod. input signal applied to Ext Mod In SMA connector

Table 27: Trigger group commands

## 5.15 SEQUENCE GROUP COMMANDS

The following set of commands provides ways to create and edit the waveform sequences in the instruments. When the instrument runs a sequence, it outputs the waveforms in the order defined in the sequence.

**Important Note:** there is only one sequence defined for an instrument. For each entry of the sequencer the number of repetitions and waveform's length are common to all channels, while Amplitude/Offset (Voltage High/Low) and waveform' shape are independent of each other.

Use the following sequence commands to define and edit a sequence:

<b>Command</b>	<b>Description</b>
SEQuence:ELEM[n]:AMPLitude[m]	Sets or returns peak to peak voltage level for sequence element n of channel m.
SEQuence:ELEM[n]:OFFset[m]	Sets or returns the offset for sequence element n of channel m.
SEQuence:ELEM[n]:VOLTage:HIGH[m]	Sets or returns the maximum level of the waveform expressed in Volts for sequence element n of channel m.
SEQuence:ELEM[n]:VOLTage:LOW[m]	Sets or returns the minimum level of the waveform expressed in Volts for sequence element n of channel m.
SEQuence:ELEM[n]:LENGth	Sets or returns the number of waveform samples for sequence element n.
SEQuence:ELEM[n]:LOOP:COUNT	Sets or returns the number of repetitions for sequence element n.
SEQuence:ELEM[n]:WAVeform[m]	Sets or returns the waveform (among those in the waveforms list) to be assigned to the sequence element n of channel m.
SEQuence:LENgth	Sets or returns the number of elements in the sequencer.
SEQuence:NEW	Creates a new sequence.
SEQuence:FOCUS	Sets which sequence element is shown on the display.
SEQuence:ELEM[n]:WAITEvent	Sets or returns the wait event type for sequence element n.
SEQuence:ELEM[n]:GOTOMode	Sets or returns the “Go To” command type for sequence element n
SEQuence:ELEM[n]:GOTOEntry	Sets or returns the target entry for the “GOTO” command for the sequence element ‘n’
SEQuence:ELEM[n]:JUMPTOMode	Sets or returns the “Jump To” command type for sequence element n
SEQuence:ELEM[n]:JUMPEvent	Sets or returns the jump event type for sequence element n.
SEQuence:ELEM[n]:JUMPTOEntry	Sets or returns the target entry index for the “Jump To” command.

SEQuence:ELEM[n]:PATTERNEvent	Sets or returns the pattern jump event type for sequence element n.
SEQuence:ELEM[n]:PATTERN	Sets or returns the pattern code value for the “Pattern Jump” command for sequence element n.
SEQuence:ELEM[n]:PATTERNJUMPTOMode	Sets or returns the “Pattern Jump” command type for sequence element n.
SEQuence:ELEM[n]:PATTERNJUMPTOEntry	Sets or returns the target entry for the “Pattern Jump” command for the sequence element ‘n’

**Table 28: Sequence group commands**

## 5.16 WAVEFORM GROUP COMMANDS

Use the following waveform commands to create and transfer waveforms between the instrument and the external controller:

Command	Description
WLIST:LIST?	Returns a list of all waveform names in the waveform list.
WLIST:NAME?	Returns the waveform name of an element which is in a specific position in the waveform list.
WLIST:SIZE?	Returns the size of the waveform list.
WLIST:WAveform:DATA?	Transfers waveform data of a waveform in waveform list to the external control program.
WLIST:WAveform:DElete	Deletes a waveform from the waveform list or all imported waveforms.
WLIST:WAveform:IMPort	Imports a waveform from internal driver or USB driver into the waveform list.
WLIST:WAveform:LENGth?	Returns the size of the specified waveform in the waveform list.
WLIST:WAveform:LMAXimum?	Returns the maximum number of waveform sample points allowed.
WLIST:WAveform:LMINimum?	Returns the minimum number of waveform sample points required for a valid waveform.
WLIST:WAveform:PREDefined?	Returns true or false based on whether the waveform is predefined (already present in waveform list by default).

Command	Description
WLIST:WAVEform:TYPE?	Returns the type of the waveform (analog or digital).

**Table 29: Waveform group commands**

## 5.17 MULTI INSTRUMENT COMMANDS

Use the following commands to synchronize multiple instrument.

The multi instrument synchronization is available on 8 channel models only.

Command	Description
MIM:CAPTure	This command captures all slave instruments
MIM:ID?	This command returns the identification number of the device in the multi-instrument chain.
MIM:CAPTured?	Returns whether the instrument has been captured by a master.
MIM:FORward?	Returns whether there is another instrument connected to the "Sync Out" port.
MIM:SLAve?	Returns whether there is another instrument connected to the "Sync In" port.
MIM:NUMber?	Returns the number of captured devices.
MIM:RELease	Releases all the captured instruments.

**Table 30: Multi-Instrument group commands and their descriptions**

## 6. COMMAND DESCRIPTIONS

### 6.1 CONTROL GROUP COMMANDS

<b>Command</b>	AWGControl:AFGSwitch (No Query Form)
<b>Description</b>	This command turns off the TrueArb application and runs the Simple AFG application
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:AFGSwitch
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AWGControl:AFGSwitch Runs the AFG application.

Table 31: AWGControl:AFGSwitch

<b>Command</b>	AWGControl:BURST
<b>Description</b>	This command sets or returns the Burst Count parameter.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:BURST {MINimum   MAXimum   DEFault   <value>} AWGControl:BURST? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt;value&gt; := &lt;NR1&gt; is the burst count</li> </ul>
<b>Returns</b>	A single <NR1> value
<b>Example</b>	AWGControl:BURST DEFault It sets the Burst Count parameter to its default value AWGControl:BURST 20 AWGControl:BURST? Might return 20.

Table 32: AWGControl:BURST

<b>Command</b>	AWGControl:CONFigure:CNUMber? (Query Only)
<b>Description</b>	This command returns the number of analog channels available on the AWG.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:CONFigure:CNUMber?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value that indicates the number of available analog channels.
<b>Example</b>	AWGControl:CONFigure:CNUMber? Might return 2.

**Table 33: AWGControl:CONFigure:CNUMber?**

<b>Command</b>	AWGControl:CONFigure:DNUMber (Query Only)
<b>Description</b>	This command returns the number of digital channels available on the AWG.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:CONFigure:DNUMber?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value that indicates the number of available digital channels.
<b>Example</b>	AWGControl:CONFigure:DNUMber? Might return 8.

**Table 34: AWGControl:CONFigure:DNUMber**

<b>Command</b>	AWGControl:DECReasing
<b>Description</b>	This command sets or returns the Sample Decreasing Strategy. The “Sample decreasing strategy” parameter defines the strategy used to adapt the waveform length to the sequencer entry length in the case where the original waveform length is longer than the sequencer entry length
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:DECReasing {DECIMation   CUTTail   CUTHead} AWGControl:DECReasing?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• DECIMation: it reduces the number of samples maintaining the waveform shape</li> </ul>

	<ul style="list-style-type: none"> <li>• CUTTail: it cuts the tail of the waveform reducing its size</li> <li>• CUTHead: it cuts the head of the waveform reducing its size.</li> </ul>
<b>Returns</b>	DECIMation   CUTTail   CUTHead
<b>Example</b>	<p>AWGControl:DECreasing CUTTail      Sets the decreasing strategy to cut tail.      AWGControl:DECreasing?      Might return DECIMation indicating that the decreasing strategy is set to decimation.</p>

**Table 35: AWGControl:DECreasing**

<b>Command</b>	AWGControl:INCreasing
<b>Description</b>	This command sets or returns the Sample Increasing Strategy. The "Sample increasing strategy" parameter defines the strategy used to adapt the waveform length to the sequencer entry length in the case where the original waveform length is shorter than the sequencer entry length.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:INCreasing {INTERpolation   RETURNzero   HOLDlast   SAMPLESMultiplication} AWGControl:INCreasing?
<b>Related Commands</b>	None
<b>Arguments</b>	INTERpolation: it performs a linear interpolation between the waveform samples RETURNzero: it fills with '0's the tail of the waveform HOLDlast: it holds the last value of the waveform SAMPLESMultiplication: it repeats the waveform samples
<b>Returns</b>	INTERpolation   RETURNzero   HOLDlast   SAMPLESMultiplication
<b>Example</b>	AWGControl:INCreasing INTERpolation Sets the increasing strategy to interpolation. AWGControl: INCreasing? Might return HOLDlast indicating that the Sample increasing strategy is set to Hold Last.

**Table 36: AWGControl:INCreasing**

<b>Command</b>	AWGControl:LENGTH:MODE
<b>Description</b>	This command sets or returns the Entry Length Strategy.

	This strategy manages the length of the sequencer entries in relationship with the length of the channel waveforms defined for each entry.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:LENGTH:MODE {ADAPTLonger   ADAPTSShorter   DEFault} AWGControl:LENGTH:MODE?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• ADAPTLonger: the length of an entry of the sequencer by default will be equal to the length of the longer channel waveform, among all analog channels, assigned to the entry.</li> <li>• ADAPTSShorter: the length of an entry of the sequencer by default will be equal to the length of the shorter channel waveform, among all analog channels, assigned to the entry.</li> <li>• DEFault:the length of an entry of the sequencer by default will be equal to the value specified in the Sequencer Item Default Length [N] parameter</li> </ul>
<b>Returns</b>	ADAPTLonger   ADAPTSShorter   DEFault
<b>Example</b>	<pre>AWGControl:LENGTH:MODE ADAPTLonger Sets the entry length strategy to "Adapt to Longer Analog Waveform".</pre> <pre>AWGControl:LENGTH:MODE? Might return DEFault.</pre>

**Table 37: AWGControl:LENGTH:MODE**

<b>Command</b>	AWGControl:RESET[:IMMediate] (No Query Form)
<b>Description</b>	<p>This command resets sequence to its default state. The sequence table will be cleared. Parameters such as sampling rate, skew time will be set to its default value.</p> <p><b>Importante Note:</b> the behaviour of this command is equivalent to *RST with the exception that before sending the AWGControl:RESET command, the AWG must be in Stopped state.</p>
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:RESET[:IMMediate]
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None

<b>Example</b>	AWGControl:RESET If the AWG is Stopped, it will reset the AWG to its default state.
----------------	--

**Table 38: AWGControl:RESET[:IMMEDIATE]**

<b>Command</b>	AWGControl:RMODE
<b>Description</b>	This command sets or returns the AWG run mode.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:RMODE {CONTinuous   BURSt   TCONTinuous   STEPped   ADVanced } AWGControl:RMODE?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• CONTinuous: each waveform will loop as written in the entry repetition parameter and the entire sequence is repeated circularly</li> <li>• BURSt: the AWG waits for a trigger event. When the trigger event occurs each waveform will loop as written in the entry repetition parameter and the entire sequence will be repeated circularly many times as written in the Burst Count[N] parameter. If you set Burst Count[N]=1 the instrument is in Single mode and the sequence will be repeated only once.</li> <li>• TCONTinuous: the AWG waits for a trigger event. When the trigger event occurs each waveform will loop as written in the entry repetition parameter and the entire sequence will be repeated circularly.</li> <li>• STEPped: the AWG, for each entry, waits for a trigger event before the execution of the sequencer entry. The waveform of the entry will loop as written in the entry repetition parameter. After the generation of an entry has completed, the last sample of the current entry or the first sample of the next entry is held until the next trigger is received. At the end of the entire sequence the execution will restart from the first entry.</li> <li>• ADVanced: it enables the “Advanced” mode. In this mode the execution of the sequence can be changed by using conditional and unconditional jumps (JUMPTO and GOTO commands) and dynamic jumps (PATTERN JUMP commands). The *RST command sets this parameter to CONTinuous.</li> </ul>
<b>Returns</b>	CONTinuous   BURSt   TCONTinuous   STEPped   ADVanced

<b>Example</b>	AWGCONTROL:RMODE STEPped Sets the AWG run mode to Stepped. AWGCONTROL:RMODE? Might return CONTinuous, indicating that the AWG run mode is set to Continuous.
----------------	---

**Table 39: AWGControl:RMODE**

<b>Command</b>	AWGControl: RSTATE? (Query Only)
<b>Description</b>	This command returns the run state of the AWG.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:RSTATE?
<b>Related Commands</b>	AWGControl:RMODE
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value. 0 indicates that the AWG has stopped. 1 indicates that the AWG is waiting for trigger. 2 indicates that the AWG is running.
<b>Example</b>	AWGCONTROL:RSTATE? Might return 0, indicating that waveform generation is stopped.

**Table 40: AWGControl:RSTATE?**

<b>Command</b>	AWGControl:RUN[:IMMediate] (No Query Form)
<b>Description</b>	This command starts the output of a sequence. This is the same to press the run button on the front-panel or display.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:RUN[:IMMediate]
<b>Related Commands</b>	AWGControl:STOP[:IMMediate]
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AWGControl:RUN Puts the AWG in the run state.

**Table 41: AWGControl:RUN[:IMMediate]**

<b>Command</b>	AWGControl:SREStore (No Query Form)
<b>Description</b>	This command opens a setup file into the AWG's setup memory.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:SREStore <cfg_name>

<b>Related Commands</b>	MMEMory:OPEN:SETup
<b>Arguments</b>	<cfg_name>::=<string>
<b>Returns</b>	None
<b>Example</b>	AWGControl:SREStore "my_configuration" Loads the setup called "my_configuration" from configurations list in 'Load From' menu.

**Table 42: AWGControl:SREStore**

<b>Command</b>	AWGControl:SSAVe (No Query Form)
<b>Description</b>	This command saves the AWG setup with waveforms.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:SSAVe <cfg_name>
<b>Related Commands</b>	MMEMory:SAVE:SETup
<b>Arguments</b>	<cfg_name>::=<string>
<b>Returns</b>	None
<b>Example</b>	AWGCONTROL:SSAVE "my_configuration" Saves the current setup into "my_configuration" that will appear in 'Save as' configurations list.

**Table 43: AWGControl:SSAVe**

<b>Command</b>	AWGControl:STOP[:IMMEDIATE] (No Query Form)
<b>Description</b>	This command stops the output of a sequence.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:STOP[:IMMEDIATE]
<b>Related Commands</b>	AWGControl:RUN[:IMMEDIATE]
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AWGControl:STOP:IMMEDIATE Stops the output of a sequence.

**Table 44: AWGControl:STOP[:IMMEDIATE]**

<b>Command</b>	AWGControl:WAITstate
<b>Description</b>	This command sets or returns the Wait Trigger On parameters. This parameter defines the behaviour of the output during the wait trigger condition in the Triggered Run Modes.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:WAITstate {FIRSTsample   LASTsample}

	AWGControl:WAITstate?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>FIRSTsample: the first waveform sample of the next entry is held until the next trigger is received</li> <li>LASTsample: the last waveform sample of the current entry is held until the next trigger is received</li> </ul>
<b>Returns</b>	FIRSTsample   LASTsample
<b>Example</b>	<pre>AWGControl:WAITstate FIRSTsample Sets the Wait Trigger On parameter to the First waveform sample. AWGControl:WAITstate? Might return FIRSTsample.</pre>

**Table 45: AWGControl:WAITstate**

<b>Command</b>	AWGControl:JUMPMODE
<b>Description</b>	This command sets or returns the Jump Mode parameter.
<b>Group</b>	Control
<b>Syntax</b>	<pre>AWGControl:JUMPMODE {AFTERrepetitions   IMMEDIATE} AWGControl:JUMPMODE?</pre>
<b>Related Commands</b>	<pre>SEQUENCE:ELEM[n]:JUMPTOMODE SEQUENCE:ELEM[n]:JUMPEVENT SEQUENCE:ELEM[n]:JUMPTOENTRY</pre>
<b>Arguments</b>	<ul style="list-style-type: none"> <li>AFTERrepetitions: the sequencer jumps to the selected entry after the completion of the current waveform repetitions.</li> <li>IMMEDIATE: the sequencer jumps as soon as possible to the selected entry, without waiting for the completion of the current waveform repetitions.</li> </ul>
<b>Returns</b>	AFTERrepetitions   IMMEDIATE
<b>Example</b>	<pre>AWGControl:JUMPMODE IMMEDIATE Sets the Jump Mode parameter to immediate jump. AWGControl:JUMPMODE? Might return IMMEDIATE.</pre>

**Table 46: AWGControl:JUMPMODE**

<b>Command</b>	AWGControl:DJStrobe (No Query Form)
<b>Description</b>	This command sends the pattern strobe event to the sequencer.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:DJStrobe <value>
<b>Related Commands</b>	SEQUENCE:ELEM[n]:PATTERN

	SEQuence:ELEM[n]:PATTERNJUMPTOMode SEQuence:ELEM[n]:PATTERNJUMPTOEntry
<b>Arguments</b>	<value> := <NR1> between 0 and 255
<b>Returns</b>	None
<b>Example</b>	AWGControl:DJStrobe 123 Sends 123 as pattern strobe event.

**Table 47: AWGControl:DJStrobe**

<b>Command</b>	AWGControl:DJump:FORce (No Query Form)
<b>Description</b>	This command allows to jump to the specified entry while the instrument is generating in Advanced mode. It is not considered while the instrument is in a wait state. It reports an error if the set entry is not present in the sequencer. It be considered as a dynamic jump.
<b>Group</b>	Control
<b>Syntax</b>	AWGControl:DJump:FORce <value>
<b>Related Commands</b>	None
<b>Arguments</b>	<value> := <NR1> between 1 and 16384 If <value> corresponds to an entry that doesn't exist the command reports an error.
<b>Returns</b>	None
<b>Example</b>	AWGControl:DJump:FORce 5000 During the generation, the instrument is forced to jump to the generation of entry 5000 regardless of the sequencer execution flow (only if entry 5000 is present in the sequencer).

**Table 48: AWGControl:DJump:FORce**

## 6.2 CALIBRATION AND DIAGNOSTIC COMMANDS

<b>Command</b>	CALibration[:ALL]
<b>Description</b>	This command does a full calibration of the AWG. In its query form, the command does a full calibration and returns a status indicating the success or failure of the operation. This command is equivalent to the *CAL? command.
<b>Group</b>	Control
<b>Syntax</b>	CALibration[:ALL] CALibration[:ALL]?
<b>Related Commands</b>	*CAL?
<b>Arguments</b>	None
<b>Returns</b>	<calibration error code> ::= <NR1> 0 indicates no error –1 indicates an error
<b>Example</b>	CALIBRATION:ALL Performs a calibration. CALIBRATION:ALL? Performs a calibration and returns results. For example, it might return 0, indicating that the calibration completed without any errors.

**Table 49: CALibration[:ALL]**

<b>Command</b>	DIAGnostic[:ALL]
<b>Description</b>	This command executes the self diagnostic procedure. The query form of this command executes the self diagnostic procedure and returns the results in the form of numeric of values of 0 for no errors or -1 for one or more tests failed.
<b>Group</b>	Control
<b>Syntax</b>	DIAGnostic[:ALL] DIAGnostic[:ALL]?
<b>Related Commands</b>	*CAL?
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value. 0 indicates no error. –1 indicates that the test failed.

<b>Example</b>	<p>DIAGNOSTIC Executes the self diagnostic procedure.</p> <p>DIAGNOSTIC? Executes the self diagnostic procedure and might return 0, indicating that there are no errors.</p>
----------------	--

**Table 50: DIAGnostic[:ALL]**

### 6.3 OUTPUT GROUP COMMANDS

<b>Command</b>	OUTPut[n]:BLOffset
<b>Description</b>	This command sets or returns the Base Line Offset parameter of the analog channel “n”.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n]:BLOffset {MINimum   MAXimum   DEFault   <Volts>} OUTPut[n]:BLOffset? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt;Volts&gt; := &lt;NRf&gt; value</li> </ul> <p>The value of n indicates the channel number.</p>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>OUTPut1:BLOffset MAXimum Sets the channel 1 Base Line Offset to the maximum value. OUTPut1:BLOffset? Might return 6V.</pre>

**Table 51: OUTPut[n]:BLOffset**

<b>Command</b>	OUTPut[n]:DElay
<b>Description</b>	This command sets or returns the Skew parameter of the analog channel “n”.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n]:DElay {MINimum   MAXimum   DEFault   <Seconds>} OUTPut[n]:DElay? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Seconds &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of n indicates the channel number.</p>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>OUTPut1:DElay 100 ns Sets the channel 1 skew to 100ns. OUTPut1:DElay? Might return 99.999E-9.</pre>

**Table 52: OUTPut[n]:DElay**

<b>Command</b>	OUTPut[n]:POLarity
<b>Description</b>	This command sets or returns the Polarity of the analog channel “n”.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n]:POLarity {NORMAl   INVerted} OUTPut[n]:POLarity?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• NORMAl: sets the polarity to positive</li> <li>• INVerted: inverts the output polarity</li> </ul> <p>The value of n indicates the channel number.</p>
<b>Returns</b>	NORMAl   INVerted
<b>Example</b>	<pre>OUTPut1:POLarity INVerted Inverts the channel 1 polarity. OUTPut1: POLarity? Might return INVerted that means the polarity is inverted.</pre>

**Table 53: OUTPut[n]:POLarity**

<b>Command</b>	OUTPut[n]:SCALe
<b>Description</b>	<p>This command sets or returns the Amplitude Scale parameter of the analog channel “n”.</p> <p>This parameter can be modified at run-time to adjust the waveform amplitude while the instrument is running and it is applied to all the waveforms contained in the sequencer. It is expressed in % and it has a range of 0% to 100%. 100% means that the waveform keeps its original amplitude.</p>
<b>Group</b>	Output
<b>Syntax</b>	<pre>OUTPut[n]:SCALe {MINimum   MAXimum   DEFault   &lt;Percentage&gt;} OUTPut[n]:SCALe? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Percentage &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of n indicates the channel number.</p>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>OUTPut1:SCALe 70. Sets the amplitude scale for the channel 1 to 70% OUTPut1:SCALe?</pre>

	Might return 70.
--	------------------

**Table 54: OUTPut[n]:SCALe**

<b>Command</b>	OUTPut[n]:SERIESIMPedance
<b>Description</b>	This command sets or returns the Output Impedance of the analog channel “n”.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n]:SERIESIMPedance {50Ohm   LOW} OUTPut[n]:SERIESIMPedance?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• 50Ohm: the output impedance is set to 50 Ohm</li> <li>• LOW: the output impedance is set to Low impedance (5 Ohm)</li> </ul> The value of n indicates the channel number.
<b>Returns</b>	<NRf>
<b>Example</b>	OUTPut1:SERIESIMPedance 50Ohm Sets the output impedance for the channel 1 to 50 Ohm. OUTPut1:SERIESIMPedance? Might return LOW that means the channel 1 output impedance is set to Low value.

**Table 55: OUTPut[n]SERIESIMPedance**

<b>Command</b>	OUTPut[n][:STATe]
<b>Description</b>	This command sets or returns the Output state of the analog channel “n”. Setting the output state of a channel to ON will switch on its analog output signal.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n][:STATe] {OFF   ON} OUTPut[n][:STATe]?
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• OFF: the selected output is disconnected from the DUT by means of a relay and the analog signal is turned off.</li> <li>• ON: the selected output is turned on</li> </ul> The value of n indicates the channel number.
<b>Returns</b>	0   1 where ‘0’ means OFF and ‘1’ means ON
<b>Example</b>	OUTPut1 ON Turns on the analog output signal and closes the output relay. OUTPut1?

	Might return 1.
--	-----------------

**Table 56: OUTPut[n]:STATe**

<b>Command</b>	DIGItals:LEVel[m]
<b>Description</b>	This command sets or returns the Voltage Level of the digital output probe (this command is available only for T3AWG3-8DIG-TTL option).
<b>Group</b>	Output
<b>Syntax</b>	DIGItals:LEVel[m] {MINimum   MAXimum   DEFault   <Volts>} DIGItals:LEVel[m]? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Volts &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of m indicates the digital probe where m=1 Digital Pod A, m=2 Digital Pod B, m=3 Digital Pod C, m=4 Digital Pod D</p>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>DIGItals:LEVel1 2.5 Sets the voltage amplitude to 2.5V for the pod A.  DIGItals:LEVel1? Might return 2.5.</pre>

**Table 57: DIGItals:LEVel[m]**

<b>Command</b>	DIGItals:NUMber
<b>Description</b>	<p>This command sets or returns the available number of the digital channels.</p> <p>The maximum number of available digital lines depends on the AWG model and on the installed license.</p> <p>There are up to 8 digital lines every 2 analog channels.</p>
<b>Group</b>	Output
<b>Syntax</b>	<pre>DIGItals:NUMber {0 2 4 6 8 10 12 14 16 18 20 22 24 26 28 30 32} DIGItals:NUMber?</pre> <p>Note: enabling the digital lines will cause a decrease of resolution in the analog output channels as shown in the user manual table (Digital Channels section).</p>

<b>Related Commands</b>	None
<b>Arguments</b>	<value> ::= <NR1> The <value> indicates the available number of the digital channels.
<b>Returns</b>	<value>
<b>Example</b>	DIGItals:NUMber 2 DIGItals:NUMber? Might returns 2.

**Table 58: DIGItals:NUMber**

<b>Command</b>	DIGItals:SKEW[m]
<b>Description</b>	This command sets or returns the Skew of the digital output probe (this command is available only for T3AWG3-8DIG-TTL option).  It sets the delay between the analog channels and the digital channels in order to de-skew the analog and digital outputs. The skew between analog/digital channels depends on the sampling frequency: the minimum skew is 1 clock cycle @ the sampling frequency.
<b>Group</b>	Output
<b>Syntax</b>	DIGItals:SKEW[m] {MINimum   MAXimum   DEFault   <Seconds>} DIGItals:SKEW[m]? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Seconds &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of m indicates the digital probe where m=1 Digital Pod A, m=2 Digital Pod B, m=3 Digital Pod C, m=4 Digital Pod D</p>
<b>Returns</b>	<NRf>
<b>Example</b>	DIGItals:SKEW1 100ns Sets the skew for the digital probe A to 100ns. DIGItals:SKEW1? Might return 100E-9.

**Table 59: DIGItals:SKEW[m]**

<b>Command</b>	DIGItals:STATe
<b>Description</b>	This command sets or returns the state of the digital outputs.

	<p>It enables or disables the available digital channels.  <b>Note:</b> if the Digital Channels number is set to '0', DIGItals:STATe ON has no effect.</p>
<b>Group</b>	Output
<b>Syntax</b>	DIGItals:STATe {OFF   ON} DIGItals:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	<p>OFF   ON</p> <ul style="list-style-type: none"> <li>• OFF: disables the digital lines</li> <li>• ON: enables the digital lines</li> </ul>
<b>Returns</b>	0   1 where '0' means OFF and '1' means ON
<b>Example</b>	<p>DIGItals:STATe ON          Enables all the available digital channels.          DIGItals:STATe?          Might returns "1" that means ON</p>

**Table 60: DIGItals:STATe**

## 6.4 DISPLAY GROUP COMMANDS

<b>Command</b>	DISPlay:FOCuS (No Query Form)
<b>Description</b>	Selects the analog output channel or digital signal (if available) that is displayed "in front" on a two/four/eight-channel instrument.
<b>Group</b>	Display
<b>Syntax</b>	DISPlay:FOCuS {CH1   CH2   CH3   CH4   CH5   CH6   CH7   CH8   DIGItals}
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• CH1   CH2   CH3   CH4   CH5   CH6   CH7   CH8 is the display page relative to the selected analog channel</li> <li>• DIGItals: digital channels display page</li> </ul>
<b>Returns</b>	None
<b>Example</b>	DISPlay:FOCuS CH2 It brings the channel 2 page to the front.

**Table 61: DISPlay:FOCuS**

<b>Command</b>	DISPlay:UNIT:VOLT (No Query Form)
<b>Description</b>	Selects the method for specifying voltage ranges. You can specify a voltage range as an amplitude and an offset or as high and low values.
<b>Group</b>	Display
<b>Syntax</b>	DISPlay:UNIT:VOLT {AMPLitudeoff   HIGHlow}
<b>Related Commands</b>	SEQunce:ELEM[n]:AMPLitude[m] SEQunce:ELEM[n]:OFFset[m] SEQunce:ELEM[n]:VOLTage:HIGH[m] SEQunce:ELEM[n]:VOLTage:LOW[m]
<b>Arguments</b>	AMPLitudeoff: specifies a voltage range as an amplitude and an offset HIGHlow: specifies a voltage range as high and low value.
<b>Returns</b>	None
<b>Example</b>	The following examples both specify a waveform voltage from 1 to 4 V for entry 1 of channel 1: DISP:UNIT:VOLT HIGH; SEQ:ELEM:VOLT:LOW 1; SEQ:ELEM:VOLT:HIGH 4;  DISP:UNIT:VOLT:AMPL; SEQ:ELEM:AMP 3;

	SEQ:ELEM:OFF 2.5;
--	-------------------

**Table 62: DISPLAY:UNIT:VOLT**

<b>Command</b>	DISPLAY[:WINDOW]:TEXT:CLEar (No Query Form)
<b>Description</b>	This command clears the text message from the display screen.
<b>Group</b>	Display
<b>Syntax</b>	DISPLAY[:WINDOW]:TEXT:CLEar
<b>Related Commands</b>	DISPLAY[:WINDOW]:TEXT[:DATA]
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	The following example writes “Hello” on the display and clears it. DISPLAY:TEXT "Hello" DISPLAY:TEXT:CLEar It clears Hello

**Table 63: DISPLAY[:WINDOW]:TEXT:CLEar**

<b>Command</b>	DISPLAY[:WINDOW]:TEXT[:DATA]
<b>Description</b>	This command sets or returns the text message displayed on the instrument screen.
<b>Group</b>	Display
<b>Syntax</b>	DISPLAY[:WINDOW]:TEXT[:DATA] <message> DISPLAY[:WINDOW]:TEXT[:DATA]?
<b>Related Commands</b>	DISPLAY[:WINDOW]:TEXT:CLEar
<b>Arguments</b>	<message> ::= <string>
<b>Returns</b>	None
<b>Example</b>	The following example writes “Hello” on the display and clears it. DISPLAY:TEXT "Hello" DISPLAY:TEXT:CLEar It clears Hello

**Table 64: DISPLAY[:WINDOW]:TEXT[:DATA]**

<b>Command</b>	HCOPY:SDUMP[:IMMEDIATE] (No Query Form)
<b>Description</b>	This command copies the current screen shot image and saves it to a specified file in the file system.
<b>Group</b>	HCopy

<b>Syntax</b>	HCOPY:SDUMP[:IMMEDIATE] <file_path>
<b>Related Commands</b>	MMEMemory:CDIRectory, MMEMemory:MSIS
<b>Arguments</b>	<file_path> must be a valid path with file name and extension. Valid extensions are: "bmp", "jpg", "jpeg", "gif", "png", "tiff". This command must be combined with the specified path with the commands MMEMemory:CDIRectory and MMEMemory:MSIS.
<b>Returns</b>	None
<b>Example</b>	MMEMemory:MSIS "D:"; HCOPY:SDUMP "my_screenshot.png"; Copies the screen shot image and creates a graphic file on the USB memory (D:) called my_screenshot.png.

**Table 65: HCOPY:SDUMP[:IMMEDIATE]**

## 6.5 LICENSE GROUP COMMANDS

<b>Command</b>	LICense:ERRor? (Query Only)
<b>Description</b>	This query-only command returns a code about license options loading operation.
<b>Group</b>	License
<b>Syntax</b>	LICense:ERRor?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value. 0 indicates no error. –1 indicates a fail condition.
<b>Example</b>	LICense:ERRor? Might return '0' that means no errors has occurred during the options loading procedure.

**Table 66: LICense:ERRor?**

<b>Command</b>	LICense:HID? (Query Only)
<b>Description</b>	This command returns the instrument HostID unique identifier.
<b>Group</b>	License
<b>Syntax</b>	LICense:HID?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<string> ::= The instrument HostID unique identifier.
<b>Example</b>	LICense:HID? Might return "T0302I20041201".

**Table 67: LICense:HID?**

<b>Command</b>	LICense: INSTall (No Query Form)
<b>Description</b>	This command accepts a license and installs it on the instrument. Restarting the instrument may be necessary to fully activate the additional capabilities.
<b>Group</b>	License
<b>Syntax</b>	LICense:INSTall <license_string>
<b>Related Commands</b>	None
<b>Arguments</b>	<license_string> ::= <string>

<b>Returns</b>	None
<b>Example</b>	LICense:INSTall <license_string> Installs license file to unit.

**Table 68: LICense: INSTall**

<b>Command</b>	LICense:LIST? (Query Only)
<b>Description</b>	This query-only command returns the license codes as a comma-separated list of string. If no license is installed an error occurs.
<b>Group</b>	License
<b>Syntax</b>	LICense:LIST?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<license_code>[,<license_code> [,<license_code>] ] ] <license_code> ::= <string>
<b>Example</b>	LICense:LIST? Might return "02f0-4fff-b528-6ef7-f501-4515-8f38-1f54"

**Table 69: LICense:LIST?**

<b>Command</b>	*OPT (Query Only)
<b>Description</b>	This command returns the installed options and application licenses for the AWG.
<b>Group</b>	License
<b>Syntax</b>	*OPT?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<opt> ::= <option_description>: <option_value> <option_description> ::= <string> <option_value> ::= <string>
<b>Example</b>	*OPT? Might return the following string: "Memory Option: 128 MSample, Digital Options: No Digital, Amplitude Option: 6 VPP, Applications Option: NO APP".

**Table 70: \*OPT**

## 6.6 MARKER GROUP COMMANDS

<b>Command</b>	MARKer:LEVel[m]
<b>Description</b>	<p>This command sets or returns the marker output 'm' Voltage Level parameter in Volts.</p> <p>The marker voltage is calculated on 50 ohm load; the minimum value is 1V@50 Ohm load and the maximum value is 2.5V@50 ohm load.</p>
<b>Group</b>	Marker
<b>Syntax</b>	<pre>MARKer:LEVel[m] {MINimum   MAXimum   DEFault   &lt;Volts&gt;} MARKer:LEVel[m]? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Volts &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of m indicates the Marker Out number: there is one marker every 2 analog channels.</p>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>MARKer:LEVel1 2.3 Sets the marker 1 level to 2.3V.  MARKer:LEVel1? MAX Might return 2.5.</pre>

Table 71: MARKer:LEVel[m]

<b>Command</b>	MARKer:MODE[m]
<b>Description</b>	This command and query sets or returns the marker output 'm' Marker Mode parameters.
<b>Group</b>	Marker
<b>Syntax</b>	<pre>MARKer:MODE[m] {FIXEDLow   FIXEDHigh   AUTOrmatic   REPLYdigital} MARKer:MODE[m]?</pre>
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• FIXEDLow: the marker level is fixed to low level</li> <li>• FIXEDHigh: the marker level is fixed to high level</li> </ul>

	<ul style="list-style-type: none"> <li>• AUTOrmatic: the marker has a behavior that depends on the Run Mode (please check Marker Settings section on TrueArb user Manual for a more in depth explanation).</li> <li>• REPLYdigital: it means that The Marker Out will behave like the Digital line 0 output. This choice is available only when the digital option is installed and the Digital Channels number is &gt; 0. The value of m indicates the Marker Out number: there is one marker every 2 analog channels.</li> </ul>
<b>Returns</b>	FIXEDLow   FIXEDHigh   AUTOrmatic   REPLYdigital
<b>Example</b>	<p>MARKer:MODE1 AUTOrmatic</p> <p>Sets the marker 1 mode to automatic. If the instrument is in Continuous, it generates a Marker pulse of the duration from 6ns to 12 ns (depending on the sampling frequency), synchronous with the analog outputs, for each sequencer entry and for each repetition.</p> <p>MARKer:MODE1?</p> <p>Might return FIXEDHigh</p>

**Table 72: MARKer:MODE[m]**

<b>Command</b>	MARKer:SKEW[m]
<b>Description</b>	<p>This command sets or returns the marker ‘m’ delay.</p> <p>It defines the skew between the marker and the analog channels. The edited value is automatically rounded to the closest value that the hardware can implement.</p>
<b>Group</b>	Marker
<b>Syntax</b>	<p>MARKer:SKEW[m] {MINimum   MAXimum   DEFault   &lt;Seconds&gt;}      MARKer:SKEW[m]? [{MINimum   MAXimum}]</p> <p><b>Important Note:</b> The maximum value you can set in the marker skew depends on the Sampling rate.</p>
<b>Related Commands</b>	None
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; Volts &gt; := &lt;NRf&gt; value</li> </ul> <p>The value of m indicates the Marker Out number.</p>
<b>Returns</b>	<NRf>
<b>Example</b>	MARKer:SKEW1 1E-9

	Sets the marker delay to 1ns MARKer:SKEW1? Might return “1E-3”
--	--

Table 73: MARKer:SKEW[m]

## 6.7 CLOCK GROUP COMMANDS

<b>Command</b>	ROSCillator
<b>Description</b>	This command sets or returns the frequency of the Reference Clock parameter.
<b>Group</b>	Clock
<b>Syntax</b>	ROSCillator {MINimum   MAXimum   DEFault   <Hertz>} ROSCillator? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	<Hertz> ::= <NRf> A single <NRf> value.
<b>Returns</b>	A single <NR3> value.
<b>Example</b>	ROSCillator 10E6 Sets a frequency of the Reference Clock to 10 MHz.

**Table 74: ROSCillator**

<b>Command</b>	AWGControl:SRATE
<b>Description</b>	This command sets or returns the sample rate for the Sampling Clock.
<b>Group</b>	Clock
<b>Syntax</b>	AWGControl:SRATE {MINimum   MAXimum   DEFault   <Hertz>} AWGControl:SRATE? [{MINimum   MAXimum}]
<b>Related Commands</b>	ROSCillator ROSCillator:SOURce
<b>Arguments</b>	<Hertz> ::= <NRf> A single <NRf> value. *RST sets this to the maximum value.
<b>Returns</b>	A single <NR3> value.
<b>Example</b>	AWGControl:SRATE 5E8 Sets the clock sample rate to 500 MHz. AWGControl:SRATE? Might return 1E+9, indicating the clock sample rate is set to 1 GHz.

**Table 75: AWGControl:SRATE**

<b>Command</b>	ROSCillator:SOURce
<b>Description</b>	This command sets the reference clock to either internal or external.
<b>Group</b>	Clock
<b>Syntax</b>	ROSCillator:SOURce {INTERNAL   EXTERNAL}

	ROSCillator:SOURce?
<b>Related Commands</b>	ROSCillator ROSCillator:SOURce
<b>Arguments</b>	<ul style="list-style-type: none"><li>INTernal: means that the reference clock is set to Internal</li><li>EXTernal: means that the reference clock is set to External</li></ul>
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce:ROSCillator:SOURce INTernal Selects the internal clock reference. ROSCillator:SOURce? Might return INT.

Table 76: ROSCillator:SOURce

## 6.8 IEEE MANDATED AND OPTIONAL GROUP COMMANDS

<b>Command</b>	*CAL? (Query Only)
<b>Description</b>	This query runs the self calibration procedure and returns a status code indicating the success or failure of self calibration. During the self calibration the AWG panel will be locked. *CAL? is equivalent to the CALibration[:ALL] command
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*CAL?
<b>Related Commands</b>	CALibration[:ALL]
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value, {0   -1}
<b>Example</b>	*CAL? Might return -1 on any failure, 0 on all pass.

Table 77: \*CAL

<b>Command</b>	*CLS (No Query Form)
<b>Description</b>	This command sets or returns the status of Event Status Enable Register (ESER). (See Status and events chapter.)
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*CLS
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*CLS Clears all the event registers and queues.

Table 78: \*CLS

<b>Command</b>	*ESE
<b>Description</b>	This command sets or returns the status of Event Status Enable Register (ESER). (See Status and events chapter.)
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*ESE <NR1> *ESE?
<b>Related Commands</b>	*CLS, *ESR?, *SRE, *STB?
<b>Arguments</b>	A single <NR1> value.
<b>Returns</b>	A single <NR1> value.

<b>Example</b>	*ESE 177 Sets the ESER to 177 (binary 10110001), which sets the PON, CME, EXE, and OPC bits. *ESE? Might return 177.
----------------	---

Table 79: \*ESE

<b>Command</b>	*ESR? (Query Only)
<b>Description</b>	This command returns the status of Standard Event Status Register (SESR). (See Status and events chapter.)
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*ESR?
<b>Related Commands</b>	*CLS, *ESE, *SRE, *STB
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	*ESR? Might return 181, which indicates that the SESR contains the binary number 10110101.

Table 80: \*ESR

<b>Command</b>	*IDN? (Query Only)
<b>Description</b>	This command returns identification information for the AWG. Refer to Std IEEE 488.2 for additional information.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*IDN?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<Manufacturer>,<Model>,<Serial Number>,<SCPI Version>,<Software Version> where: <ul style="list-style-type: none"> <li>- &lt;Manufacturer&gt;::= ACTIVE TECHNOLOGIES,</li> <li>- &lt;Model&gt;::=T3AWG3X5X,</li> <li>- &lt;Serial Number&gt;::=indicates an actual serial number,</li> <li>- &lt;SCPI Version&gt;::=SCPI:1999.0,</li> <li>- &lt;Software Version&gt;::={AFG   AWG}.{X.X.X} where: <ul style="list-style-type: none"> <li>• AFG   AWG specifies the application (AFG = Simple Function Generator, AWG = True Arb),</li> <li>• X.X.X. specifies the revision.</li> </ul> </li> </ul>

<b>Example</b>	*IDN? Example returns: ACTIVE TECHNLOGIES,T3AWG3352,T03020I18450099,SCPI:1999.0, SV:AWG.3.2.19.
----------------	--

**Table 81: \*IDN?**

<b>Command</b>	*OPC
<b>Description</b>	This command causes the AWG to sense the internal flag referred to as the “No-Operation-Pending” flag. The command sets bit 0 in the Standard Event Status Register when pending operations are complete. The query form returns a “1” when the last overlapping command operation is finished.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*OPC *OPC?
<b>Related Commands</b>	*WAI
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	*OPC? Returns 1 to indicate that the last issued overlapping command is finished.

**Table 82: \*OPC**

<b>Command</b>	*RST (No Query Form)
<b>Description</b>	This command resets the AWG to its default state. The AWG will be stopped.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*RST
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*RST Resets the AWG.

**Table 83: \*RST**

<b>Command</b>	*SRE
----------------	------

<b>Description</b>	This command sets or returns the bits in the Service Request Enable register. (See Status and events chapter.)
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*SRE <enable_value> *SRE?
<b>Related Commands</b>	*CLS, *ESE, *ESR?, *STB?
<b>Arguments</b>	A single <NR1> value.
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	*SRE 48 Sets the bits in the SRER to the binary value 00110000. *SRE? Might return a value of 32, showing that the bits in the SRER have the binary value 00100000.

**Table 84: \*SRE**

<b>Command</b>	*TRG (No Query Form)
<b>Description</b>	This command generates a trigger event. This is equivalent to press and release the trigger button on the front panel.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*TRG
<b>Related Commands</b>	TRIGger[:IMMediate], AWGControl:RMODe
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*TRG Generates a trigger event.

**Table 85: \*TRG**

<b>Command</b>	*TST? (Query Only)
<b>Description</b>	This command executes the Self Diagnostic procedure.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*TST?
<b>Related Commands</b>	DIAGnostic[:IMMediate], DIAGnostic:DATA?, DIAGnostic:RESUlt?
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value.

	A returned value of 0 indicates no error.
<b>Example</b>	*TST? M Might return -1, indicating that the Self Diagnostic procedure failed.

**Table 86: \*TST?**

<b>Command</b>	*WAI (No Query Form)
<b>Description</b>	This command is used to ensure that the previous command is complete before the next command is issued.
<b>Group</b>	IEEE Mandated and Optional Group Command
<b>Syntax</b>	*WAI
<b>Related Commands</b>	*OPC
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*WAI Prevents the instrument from executing any further commands or queries until all pending commands that generate an OPC message are complete.

**Table 87: \*WAI**

## 6.9 PARAMETRIC WAVEFORMS COMMANDS

<b>Command</b>	PW:CREATE (No Query Form)
<b>Description</b>	This command creates a new parametric waveform in waveform list. If the name of the waveform to be created already exists in waveforms list, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:CREATE <pw_name>,[{NOTPredefined   PREdefined}],<description>
<b>Related Commands</b>	PW:DELETE
<b>Arguments</b>	<pw_name>,[{NOTPredefined   PREdefined}],<description> where: <"pw_name"> ::= <string> is the name of the new parametric wave, NOTPredefined   PREdefined: specifies if the new parametric wave will be Predefined or not; if omitted, the new parametric wave will be <u>not</u> predefined. <"description">: allows to insert a brief description of the wave.
<b>Returns</b>	None
<b>Example</b>	PW:CREATE "My_Pwave_1",PREdefined,"my scenario 1" Creates the predefined parametric wave 'My_Pwave_1', the description 'my scenario 1' is associated with this wave.  PW:CREATE "My_Pwave_2", Creates the not-predefined parametric wave 'My_Pwave_2' without any description.

**Table 88: PW:CREATE**

<b>Command</b>	PW:DELETE (No Query Form)
<b>Description</b>	This command deletes a specific parametric waveform or all parametric waveforms present in waveforms list. If the name of the waveform to be deleted is not present in the waveforms list, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:DELETE {ALL   <pw_name>}
<b>Related Commands</b>	PW:CREATE
<b>Arguments</b>	ALL   <pw_name> where:

	<"pw_name"> ::= <string> is the name of the waveform to be deleted, ALL : deletes all parametric waves from the waveforms list.
<b>Returns</b>	None
<b>Example</b>	PW:DELETE “My_Pwave_1” Deletes from the waveforms list the parametric wave ‘My_Pwave_1’.

**Table 89: PW:DELETE**

<b>Command</b>	PW: DUPLICATE (No Query Form)
<b>Description</b>	This command creates a copy of a target wave with a specified name. If the target wave is not present in the waveforms list, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW: DUPLICATE <target_name>,<duplication_name>
<b>Related Commands</b>	PW:CREATE
<b>Arguments</b>	<target_name>,<duplication_name> where: <" target_name"> ::= <string> is the name of the waveform to duplicate, <"duplication_name"> ::= <string> is the new name of the duplicated wave.
<b>Returns</b>	None
<b>Example</b>	PW:DUPLICATE “My_Wave_1”,“Duplicated_Wave” Creates a copy of ‘My_Wave_1’, the name of this new waveform is ‘Duplicated_Wave’.

**Table 90: PW:DUPLICATE**

<b>Command</b>	PW:RENAME (No Query Form)
<b>Description</b>	This command allows to rename a specified waveform of the waveforms list. If the waveform is not present in the waveforms list, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:RENAME <old_name>,<new_name>

<b>Related Commands</b>	PW:CREATE
<b>Arguments</b>	<old_name>,<new_name> where: <"old_name"> ::= <string> is the name of a waveform present in the waveform list. <"new_name"> ::= <string> is the new name of the wave.
<b>Returns</b>	None
<b>Example</b>	PW:RENAME "My_Wave_1","Standard_Wave_1" Changes the name of 'My_Wave_1' waveform in 'Standard_Wave_1'.

**Table 91: PW:RENAME**

<b>Command</b>	PW:TYPe
<b>Description</b>	This command sets or queries the type of the parametric waveform. If the specified waveform has not been previously created, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:TYPe <pw_name>,{SINe   PULse   SWEep   SINc   EXP   PRBs   SQUare   MULTitone}, PW:TYPe? <pw_name>
<b>Related Commands</b>	PW:CREATE
<b>Arguments</b>	<"pw_name"> ::= <string> is the name of a parametric waveform already created in the waveform list. SINe   PULse   SWEep   SINc   EXP   PRBs   SQUare   MULTitone
<b>Returns</b>	SINe   PULse   SWEep   SINc   EXP   PRBs   SQUare   MULTitone
<b>Example</b>	PW:TYPe "My_Pwave_1",PRBs Sets the parameter Type of 'My_Pwave_1' waveform as PRBS. PW:TYPe? "My_Pwave_1" Returns PRBs.

**Table 92: PW:TYPe**

<b>Command</b>	PW:[COMMON:]CYCles
<b>Description</b>	This command sets or queries the parameter 'Cycles' of a parametric waveform. The parameter 'Cycles' is present only for parametric waveforms whose type is Sine, Pulse, Exponential or Square.

	It's not possible to modify the value of 'Cycles' if the 'Auto Calc Option' parameter is set as 'Cycles' or 'Length & Cycles'.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:[COMMON:]CYCles <pw_name>,{MINimum   MAXimum   DEFault   <value>}, PW:[COMMON:]CYCles? <pw_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pw_name"&gt; ::= &lt;string&gt; is the name of the parametric waveform whose number of cycles you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum number of cycles.</li> <li>• MAXimum sets or queries the maximum number of cycles.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;value&gt; := &lt;NR1&gt; is the number of cycles.</li> </ul>
<b>Returns</b>	<NR1>
<b>Example</b>	<pre>PW:COMMON:CYCles "My_Pwave_Pulse",10 Sets the cycles number of 'My_Pwave_Pulse' waveform to 10. PW:COMMON:CYCles? "My_Pwave_Pulse",MINimum Might return 1.</pre>

**Table 93: PW:[COMMON:]CYCles**

<b>Command</b>	PW:[COMMON:]PHASE
<b>Description</b>	<p>This command sets or queries the parameter 'Phase' of a parametric waveform.</p> <p>The parameter 'Phase' is present only for parametric waveforms whose type is Sine.</p> <p>For the 'Multitone' parametric waveform use &lt;Deg&gt; field of PW:MULTit:ADD command or PW:MULTit:TONE[k]:PHASE command to set the phase of a single tone.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:[COMMON:]PHASE <pw_name>,{MINimum   MAXimum   DEFault   <Deg>}, PW:[COMMON:]PHASE? <pw_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pw_name"&gt; ::= &lt;string&gt; is the name of the parametric waveform whose value of phase you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> </ul>

	<ul style="list-style-type: none"> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt; Deg &gt; := &lt;NRf&gt; degrees of phase.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:COMMON:PHASE “My_Pwave_Sine”,50  Sets the phase of ‘My_Pwave_Sine’ waveform to 50°.</p> <p>PW:COMMON:PHASE? “My_Pwave_Sine”,MAXimum  Returns 360.000.</p>

**Table 94: PW:[COMMON:]PHASE**

<b>Command</b>	PW:[COMMON:]FREquency
<b>Description</b>	<p>This command sets or queries the parameter ‘Frequency’ of a parametric waveform.</p> <p>The parameter ‘Frequency’ is present only for parametric waveforms whose type is Sine, Pulse or Square.</p> <p>For the ‘Multitone’ parametric waveform use &lt;hertz&gt; field of PW:MULTit:ADD command to set the frequency of a single tone.</p> <p><b>Note:</b> frequency and period are dual parameters of the same field; once this command has been launched, the parameter is automatically switched to ‘Frequency [Hz]’.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<p>PW:[COMMON:]FREquency  &lt;pw_name&gt;,{MINimum   MAXimum   DEFault   &lt;Hertz&gt;},  PW:[COMMON:]FREquency? &lt;pw_name&gt;,[{MINimum   MAXimum}]</p>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;“pw_name”&gt; ::= &lt;string&gt; is the name of the parametric waveform whose value of frequency you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Hertz&gt; := &lt;NRf&gt; frequency of parametric waveform.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:COMMON:FREquency “My_Pwave_Square”,20E6  Sets the frequency of ‘My_Pwave_Square’ waveform to 20 Mhz.</p> <p>PW:COMMON:FREquency? “My_Pwave_Square”  Might return 20000000.</p>

**Table 95: PW:[COMMON:]FREquency**

<b>Command</b>	PW:[COMmon:]PERiod
<b>Description</b>	<p>This command sets or queries the parameter ‘Period’ of a parametric waveform.</p> <p>The parameter ‘Period’ is present only for parametric waveforms whose type is Sine, Pulse or Square.</p> <p><b>Note:</b> frequency and period are dual parameters of the same field; once this command has been launched, the parameter is automatically switched to ‘Period [s]’.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<pre>PW:[COMmon:]PERiod &lt;pw_name&gt;,{MINimum   MAXimum   DEFault   &lt;Seconds&gt;}, PW:[COMmon:]PERiod? &lt;pw_name&gt;,[{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;“pw_name”&gt; ::= &lt;string&gt; is the name of the parametric waveform whose value of period you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; period of parametric waveform.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>PW:COMMON:PERiod "My_Pwave_Pulse",2us Sets the period of 'My_Pwave_Pulse' waveform to 2 us.</pre> <pre>PW:COMMON:PERiod? "My_Pwave_Pulse" Might return 0.000002000.</pre>

**Table 96: PW:[COMmon:]PERiod**

<b>Command</b>	PW:[COMmon:]LENgth
<b>Description</b>	<p>This command sets or queries the parameter ‘Length’ (number of samples) of a parametric waveform.</p> <p>The parameter ‘Length’ is present in all type of parametric waveforms but for the Multitone type, only the query of the command is available.</p> <p><b>Note 1:</b> length and duration are dual parameters of the same field for the parametric waveforms whose type is Sweep, Sinc, Exponential or Prbs;</p>

	once this command has been launched, the parameter is automatically switched to 'Length [N]'. <b>Note 2:</b> for Sine, Pulse and Square types, it's not possible to modify the value of 'Length' if the 'Auto Calc Option' parameter is set as 'Length' or 'Length & Cycles'.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:[COMMON:]LENgth <pw_name>,{MINimum   MAXimum   DEFault   <value>}, PW:[COMMON:]LENgth? <pw_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPe
<b>Arguments</b>	<"pw_name"> ::= <string> is the name of the parametric waveform whose value of samples you want to set or query. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;value&gt; := &lt;NR1&gt; number of samples.</li> </ul>
<b>Returns</b>	<NR1>
<b>Example</b>	PW:COMMON:LENgth "My_Pwave_Pulse",100 Sets the length of 'My_Pwave_Pulse' waveform to 100.  PW:COMMON:LENgth? "My_Pwave_Pulse" Returns 100.

**Table 97: PW:[COMMON:]LENgth**

<b>Command</b>	PW:[COMMON:]DURation
<b>Description</b>	This command sets or queries the parameter 'Duration' of a parametric waveform. The parameter 'Duration' is present only for parametric waveforms whose type is Sweep, Sinc, Exponential or Prbs. The value of this parameter will be automatically rounded to the closest time interval that the instrument is able to generate. <b>Note:</b> length and duration are dual parameters of the same field; once this command has been launched, the parameter is automatically switched to 'Duration [s]'.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:[COMMON:]DURation <pw_name>,{MINimum   MAXimum   DEFault   <Seconds>},

	PW:[COMmon:]DURation? <pw_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pw_name"&gt; ::= &lt;string&gt; is the name of the parametric waveform whose duration you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; value of duration.</li> </ul>
<b>Returns</b>	<NR1>
<b>Example</b>	<p>PW:COMMON:DURATION "My_Pwave_Sinc",500ns  Sets the duration of 'My_Pwave_Sinc' waveform to 500 ns.</p> <p>PW:COMMON:DURATION? "My_Pwave_Sinc"  Returns 506.666E-9.</p>

**Table 98: PW:[COMmon:]DURation**

<b>Command</b>	PW:[COMmon:]SRate
<b>Description</b>	<p>This command sets or queries the parameter 'Sampling Rate' of a parametric waveform.</p> <p>The parameter 'Sampling Rate' is present in all type of parametric waveforms.</p> <p>This parameter is independent of the 'Sampling Clock' value (see AW-GControl:SRATE command).</p> <p><b>Note :</b> for Sine, Pulse and Square types, it's not possible to modify the value of 'Sampling Rate' if the 'Auto Calc Option' parameter is set as Sampling Rate.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<p>PW:[COMmon:]SRate  &lt;pw_name&gt;,{MINimum   MAXimum   DEFault   &lt;Hertz&gt;},  PW:[COMmon:]SRate? &lt;pw_name&gt;,[{MINimum   MAXimum}]</p>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pw_name"&gt; ::= &lt;string&gt; is the name of the parametric waveform whose value of sampling rate you want to set or query.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> </ul>

	<ul style="list-style-type: none"> <li>• &lt;Hertz&gt; := &lt;NRf&gt; value of sampling rate.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:COMMON:SRate "My_Pwave_Pulse",500E6  Sets the sampling rate of 'My_Pwave_Pulse' waveform to 500 Mhz.</p> <p>PW:COMMON:SRate? "My_Pwave_Pulse"  Returns 500000000.</p>

**Table 99: PW:[COMMON]:SRate**

<b>Command</b>	PW:[COMMON]:ACOption
<b>Description</b>	This command sets or queries the strategy of 'Auto Calc Option'. This parameter is not present in parametric waveforms whose type is Sweep, Sinc, Exp, Prbs or Multitone.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<p>PW:[COMMON]:ACOption  &lt;pw_name&gt;,{LENgth   SPRate   CYCles   LENGTHCycles},  PW:[COMMON]:ACOption? &lt;pw_name&gt;</p>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pw_name"&gt; ::= &lt;string&gt; is the name of the parametric waveform whose 'Auto Calc Option' parameter you want to set or query.</p> <p>LENgth   SPRate   CYCles   LENGTHCycles where:</p> <ul style="list-style-type: none"> <li>• LENgth means Length,</li> <li>• SPRate means Sampling Rate,</li> <li>• CYCles means Cycles,</li> <li>• LENGTHCycles means Length &amp; Cycles.</li> </ul>
<b>Returns</b>	LENgth   SPRate   CYCles   LENGTHCycles
<b>Example</b>	<p>PW:COMMON:ACOption "My_Pwave_Pulse",SPRate  Sets 'Sampling Rate' strategy for Auto Calc Option of the 'My_Pwave_Pulse' parametric waveform.</p> <p>PW:COMMON:ACOption? "My_Pwave_Pulse"  Might return SPRate.</p>

**Table 100: PW:[COMMON]:ACOption**

<b>Command</b>	PW:[COMMON]:WRAPAround
----------------	------------------------

<b>Description</b>	This command sets or queries the status of 'Wrap Around' parameter. This parameter is not present in parametric waveforms whose type is Sweep, Sinc, Exp, Prbs or Multitone.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:[COMMON:]WRAPAround <pw_name>,{ON   OFF   0   1}, PW:[COMMON:]WRAPAround? <pw_name>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"pw_name"> ::= <string> is the name of the parametric waveform whose 'Wrap Around' parameter you want to set or query. <ul style="list-style-type: none"> <li>• ON   1 enables the Wrap Around option for the specified waveform.</li> <li>• OFF   0 disables the Wrap Around option for the specified waveform.</li> </ul>
<b>Returns</b>	0 means OFF, 1 means ON
<b>Example</b>	PW:COMMON:WRAPAround "My_Pwave_Pulse",ON Turns on the Wrap Around switch of 'My_Pwave_Pulse' parametric waveform.  PW:COMMON:WRAPAround? "My_Pwave_Pulse" Might return 1.

**Table 101: PW:[COMMON:]WRAPAround**

<b>Command</b>	PW:PULse:FALltime
<b>Description</b>	This command sets or queries the Fall Time of a parametric Pulse waveform. Note that the value is about the falling edge between 10% and 90%. If the type of the parametric waveform is different from Pulse, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:PULse:FALltime <pulse_name>,{MINimum   MAXimum   DEFault   <Seconds>}, PW:PULse:FALltime? <pulse_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"pulse_name"> ::= <string> is the name of the parametric pulse waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> </ul>

	<ul style="list-style-type: none"> <li>• &lt;Seconds&gt; := &lt;NRf&gt; value of Fall Time.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:PULse:FALLtime "My_Pwave_Pulse",5ns  Sets the Fall Time of 'My_Pwave_Pulse' parametric waveform to 5 ns.</p> <p>PW:PULse:FALLtime? "My_Pwave_Pulse"  Might return 5.000E-9.</p>

**Table 102: PW:PULse:FALLtime**

<b>Command</b>	PW:PULSE:RISetime
<b>Description</b>	<p>This command sets or queries the Rise Time of a parametric Pulse waveform.</p> <p>Note that the value is about the rising edge between 10% and 90%. If the type of the parametric waveform is different from Pulse, this command reports an error.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<p>PW:PULSE:RISetime  &lt;pulse_name&gt;,{MINimum   MAXimum   DEFault   &lt;Seconds&gt;},  PW:PULSE:RISetime? &lt;pulse_name&gt;,[{MINimum   MAXimum}]</p>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"pulse_name"&gt; ::= &lt;string&gt; is the name of the parametric pulse waveform.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; value of Rise Time.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:PULSE:RISetime "My_Pwave_Pulse",2ns  Sets the Rise Time of 'My_Pwave_Pulse' parametric waveform to 2 ns.</p> <p>PW:PULSE:RISetime? "My_Pwave_Pulse"  Might return 2.000E-9.</p>

**Table 103: PW:PULse:RISetime**

<b>Command</b>	PW:PULSE:DUTycycle
----------------	--------------------

<b>Description</b>	This command sets or queries the Duty Cycle of a parametric Pulse waveform. <b>Note 1:</b> duty cycle and pulse width are dual parameters of the same field; once this command has been launched, the parameter is automatically switched to 'Duty Cycle [%]'. <b>Note 2:</b> if the type of the parametric waveform is different from Pulse, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:PULse:DUTycycle <pulse_name>,{MINimum   MAXimum   DEFault   <Percentage>}, PW:PULse:DUTycycle? <pulse_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"pulse_name"> ::= <string> is the name of the parametric pulse waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Percentage&gt; := &lt;NR2&gt; is the value of duty cycle.</li> </ul>
<b>Returns</b>	<NR2>
<b>Example</b>	PW:PULse:DUTycycle "My_Pwave_Pulse",30 Sets the duty cycle of 'My_Pwave_Pulse' parametric waveform to 30%.  PW:PULse:DUTycycle? "My_Pwave_Pulse" Might return 30.000.

**Table 104: PW:PULse:DUTycycle**

<b>Command</b>	PW:PULse:PWldth
<b>Description</b>	This command sets or queries the Pulse Width parameter of a parametric Pulse waveform. <b>Note 1:</b> duty cycle and pulse width are dual parameters of the same field; once this command has been launched, the parameter is automatically switched to 'Pulse Width [s]'. <b>Note 2:</b> if the type of the parametric waveform is different from Pulse, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:PULse:PWldth <pulse_name>,{MINimum   MAXimum   DEFault   <Seconds>},

	PW:PULse:PWlDth? <pulse_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"pulse_name"> ::= <string> is the name of the parametric pulse waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; is the value of the pulse width.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:PULse:PWlDth "My_Pwave_Pulse",200ns Sets the pulse width of 'My_Pwave_Pulse' parametric waveform to 200 ns.  PW:PULse:PWlDth? "My_Pwave_Pulse" Might return 0.0000002000.

**Table 105: PW:PULse:PWlDth**

<b>Command</b>	PW:PULse:PDElay
<b>Description</b>	This command sets or queries the Pulse Delay parameter of a parametric Pulse waveform. <b>Note:</b> if the type of the parametric waveform is different from Pulse, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:PULse:PDElay <pulse_name>,{MINimum   MAXimum   DEFault   <Seconds>}, PW:PULse:PDElay? <pulse_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"pulse_name"> ::= <string> is the name of the parametric pulse waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; is the value of the pulse delay.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:PULse:PDElay "My_Pwave_Pulse",33ns Sets the pulse delay of 'My_Pwave_Pulse' parametric waveform to 33 ns.  PW:PULse:PDElay? "My_Pwave_Pulse"

	Might return 0.000000033000.
--	------------------------------

Table 106: PW:PULse:PDElay

<b>Command</b>	PW:SWEep:STArtfreq
<b>Description</b>	This command sets or queries the Start Frequency parameter of a parametric Sweep waveform. <b>Note:</b> if the type of the parametric waveform is different from Sweep, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SWEep:STArtfreq <sweep_name>,{MINimum   MAXimum   DEFault   <Hertz>}, PW:SWEep:STArtfreq? <sweep_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"sweep_name"> ::= <string> is the name of the parametric sweep waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Hertz&gt; := &lt;NRf&gt; is the value of the Start Frequency.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:SWEep:STArtfreq "My_Pwave_Sweep",500E3 Sets the Start Frequency of 'My_Pwave_Sweep' parametric waveform to 500 khz.  PW:SWEep:STArtfreq? "My_Pwave_Sweep" Might return 500.000E3.

Table 107: PW:SWEep:STArtfreq

<b>Command</b>	PW:SWEep:STOPfreq
<b>Description</b>	This command sets or queries the Stop Frequency parameter of a parametric Sweep waveform. <b>Note:</b> if the type of the parametric waveform is different from Sweep, this command reports an error.
<b>Group</b>	Parametric Waveforms

<b>Syntax</b>	PW:SWEep:STOpfreq <sweep_name>,{MINimum   MAXimum   DEFault   <Hz>}, PW:SWEep:STOpfreq? <sweep_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPe
<b>Arguments</b>	<p>&lt;"sweep_name"&gt; ::= &lt;string&gt; is the name of the parametric sweep waveform.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Hz&gt; := &lt;NRf&gt; is the value of the Stop Frequency.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>PW:SWEep:STOpfreq "My_Pwave_Sweep",5E6 Sets the Stop Frequency of 'My_Pwave_Sweep' parametric waveform to 5 Mhz.</pre> <pre>PW:SWEep:STOpfreq? "My_Pwave_Sweep" Might return 5.000E6.</pre>

**Table 108: PW:SWEep:STOpfreq**

<b>Command</b>	PW:SWEep:MODe
<b>Description</b>	This command sets or queries the sweep mode of a parametric Sweep waveform. <b>Note:</b> if the type of the parametric waveform is different from Sweep, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SWEep:MODe <sweep_name>,{LINear   LOGarithmic}, PW:SWEep:MODe? <sweep_name>
<b>Related Commands</b>	PW:CREATE, PW:TYPe
<b>Arguments</b>	<p>&lt;"sweep_name"&gt; ::= &lt;string&gt; is the name of the parametric sweep waveform.</p> <ul style="list-style-type: none"> <li>• LINear sets a linear sweep mode.</li> <li>• LOGarithmic sets a logarithmic sweep mode.</li> </ul>
<b>Returns</b>	LINear   LOGarithmic
<b>Example</b>	PW:SWEep:MODe "My_Pwave_Sweep",LOGarithmic

	Sets a logarithmic sweep mode for 'My_Pwave_Sweep' parametric waveform.  PW:SWEep:MODE? "My_Pwave_Sweep" Might return LOGarithmic.
--	---

Table 109: PW:SWEep:MODE

<b>Command</b>	PW:SINC:PEAkpos
<b>Description</b>	This command sets or queries the Peak Position (expressed as a percentage) of a parametric Sinc waveform.  <b>Note:</b> if the type of the parametric waveform is different from Sinc, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SINC:PEAkpos <sinc_name>,{MINimum   MAXimum   DEFault   <Percentage>}, PW:SINC:PEAkpos? <sinc_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"sinc_name"> ::= <string> is the name of the parametric sinc waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Percentage&gt; ::= &lt;NRf&gt; is the value of the Peak Position.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:SINC:PEAkpos "My_Pwave_Sinc",70 Sets the peak position of 'My_Pwave_Sinc' parametric waveform to 70%.  PW:SINC:PEAkpos? "My_Pwave_Sinc",MAXimum Might return 100.0.

Table 110: PW:SINC:PEAkpos

<b>Command</b>	PW:SINC:LOBewidth
<b>Description</b>	This command sets or queries the Lobe Width (expressed as a percentage) of a parametric Sinc waveform.

	<b>Note:</b> if the type of the parametric waveform is different from Sinc, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SINC:LOBewidth <sinc_name>,{MINimum   MAXimum   DEFault   <Percentage>}, PW:SINC:LOBewidth? <sinc_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"sinc_name"> ::= <string> is the name of the parametric sinc waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Percentage&gt; := &lt;NRF&gt; is the value of the Lobe Width.</li> </ul>
<b>Returns</b>	<NRF>
<b>Example</b>	PW:SINC:LOBewidth "My_Pwave_Sinc",25 Sets the lobe width of 'My_Pwave_Sinc' parametric waveform to 25%.  PW:SINC:LOBewidth? "My_Pwave_Sinc" Might return 25.0.

**Table 111: PW:SINC:LOBewidth**

<b>Command</b>	PW:EXP:TIMEconst
<b>Description</b>	This command sets or queries the Time Constant of a parametric Exponential waveform. <b>Note:</b> if the type of the parametric waveform is different from Exp, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:EXP:TIMEconst <exp_name>,{MINimum   MAXimum   DEFault   <Seconds>} PW:EXP:TIMEconst? <exp_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"exp_name"> ::= <string> is the name of the parametric exponential waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRF&gt; is the value of the Time Constant.</li> </ul>

<b>Returns</b>	<NRf>
<b>Example</b>	<pre>PW:EXP:TIMEconst "My_Pwave_Exp",1.2E-6</pre> <p>Sets the time constant of 'My_Pwave_Exp' parametric waveform to 1.2 us.</p> <pre>PW:EXP:TIMEconst? "My_Pwave_Exp"</pre> <p>Might return 1.200000E-6.</p>

**Table 112: PW:EXP:TIMEconst**

<b>Command</b>	PW:EXP:MODE
<b>Description</b>	<p>This command sets or queries the mode (Rise or Decay) of a parametric Exponential waveform.</p> <p><b>Note:</b> if the type of the parametric waveform is different from Exp, this command reports an error.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<pre>PW:EXP:MODE &lt;exp_name&gt;,{RISe   DECay},</pre> <pre>PW:EXP:MODE? &lt;exp_name&gt;</pre>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"exp_name"&gt; ::= &lt;string&gt; is the name of the parametric exponential waveform.</p> <ul style="list-style-type: none"> <li>• RISe means rise mode,</li> <li>• DECay means decay mode.</li> </ul>
<b>Returns</b>	RISe   DECay
<b>Example</b>	<pre>PW:EXP:MODE "My_Pwave_Exp",RISe</pre> <p>Sets the rise mode for the 'My_Pwave_Exp' parametric waveform.</p> <pre>PW:EXP:MODE? "My_Pwave_Exp"</pre> <p>Might return RISe.</p>

**Table 113: PW:EXP:MODE**

<b>Command</b>	PW:PRBs:TYPE
<b>Description</b>	<p>This command sets or queries the Prbs order (or type) of a parametric Prbs waveform.</p> <p><b>Note:</b> if the type of the parametric waveform is different from Prbs, this command reports an error.</p>
<b>Group</b>	Parametric Waveforms

<b>Syntax</b>	PW:PRBs:TYPe <prbs_name>,{7 9 11 15 23 31}, PW:PRBs:TYPe? <prbs_name>
<b>Related Commands</b>	PW:CREATE, PW:TYPe
<b>Arguments</b>	<"prbs_name"> ::= <string> is the name of the parametric prbs waveform. 7 9 11 15 23 31 where: <ul style="list-style-type: none"><li>• 7 means type PRBS-7,</li><li>• 9 means type PRBS-9,</li><li>• 11 means type PRBS-11,</li><li>• 15 means type PRBS-15,</li><li>• 23 means type PRBS-23,</li><li>• 31 means type PRBS-31.</li></ul>
<b>Returns</b>	7 9 11 15 23 31
<b>Example</b>	PW:PRBs:TYPe "My_Pwave_Prbs",15 Sets the type PRBS-15 for the 'My_Pwave_Prbs' parametric waveform.  PW:PRBs:TYPe? "My_Pwave_Prbs" Might return 15.

Table 114: PW:PRBs:TYPe

<b>Command</b>	PW:SQUare:FALLtime
<b>Description</b>	This command sets or queries the Fall Time of a parametric Square waveform.  Note that the value is about the falling edge between 10% and 90%. If the type of the parametric waveform is different from Square, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SQUare:FALLtime <square_name>,{MINimum   MAXimum   DEFault   <Seconds>} PW:SQUare:FALLtime? <square_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPe
<b>Arguments</b>	<"square_name"> ::= <string> is the name of the parametric square waveform. <ul style="list-style-type: none"><li>• MINimum sets or queries the minimum value of param.</li><li>• MAXimum sets or queries the maximum value of param.</li><li>• DEFault: sets the parameter to the default value.</li></ul>

	<ul style="list-style-type: none"> <li>• &lt;Seconds&gt; := &lt;NRf&gt; value of Fall Time.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:SQUare:FALLtime "My_Pwave_Square",2ns          Sets the Fall Time of 'My_Pwave_Square' parametric waveform to 2 ns.</p> <p>PW:SQUare:FALLtime? "My_Pwave_Square"          Might return 2.000E-9.</p>

**Table 115: PW:SQUare:FALLtime**

<b>Command</b>	PW:SQUare:RISetime
<b>Description</b>	<p>This command sets or queries the Rise Time of a parametric Square waveform.</p> <p>Note that the value is about the rising edge between 10% and 90%.</p> <p>If the type of the parametric waveform is different from Square, this command reports an error.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	<p>PW:SQUare:RISetime          &lt;square_name&gt;,{MINimum   MAXimum   DEFault   &lt;Seconds&gt;},          PW:SQUare:RISetime? &lt;square_name&gt;,[{MINimum   MAXimum}]</p>
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<p>&lt;"square_name"&gt; ::= &lt;string&gt; is the name of the parametric square waveform.</p> <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt; Seconds&gt; := &lt;NRf&gt; value of Rise Time.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<p>PW:SQUare:RISetime "My_Pwave_Square",2ns          Sets the Rise Time of 'My_Pwave_Square' parametric waveform to 2 ns.</p> <p>PW:SQUare:RISetime? "My_Pwave_Square"          Might return 2.000E-9.</p>

**Table 116: PW:SQUare:RISetime**

<b>Command</b>	PW:SQUare:PDElay
----------------	------------------

<b>Description</b>	This command sets or queries the Pulse Delay parameter of a parametric Square waveform. <b>Note:</b> if the type of the parametric waveform is different from Square, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:SQUare:PDElay <square_name>,{MINimum   MAXimum   DEFault   <Seconds>} PW:SQUare:PDElay? <square_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE
<b>Arguments</b>	<"square_name"> ::= <string> is the name of the parametric square waveform. <ul style="list-style-type: none"> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Seconds&gt; := &lt;NRf&gt; is the value of the pulse delay.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:SQUare:PDElay "My_Pwave_Square",10ns Sets the pulse delay of 'My_Pwave_Square' parametric waveform to 10 ns.  PW:SQUare:PDElay? "My_Pwave_Square" Might return 0.00000010000.

**Table 117: PW:SQUare:PDElay**

<b>Command</b>	PW:MULTit:ADD (No Query Form)
<b>Description</b>	This command creates a new sinusoidal tone with a specified frequency, amplitude and phase in a parametric Multitone waveform.  <b>Note 1:</b> if the type of the parametric waveform is different from Multitone, this command reports an error. <b>Note 2:</b> in a parametric multitone waveform it is possible to insert up to a maximum of 10 tones.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:ADD <mtone_name>,{MINimum   MAXimum   DEFault   <Hertz>},{MINimum   MAXimum   DEFault   <Volts>},{MINimum   MAXimum   DEFault   <Gradients>}
<b>Related Commands</b>	PW:CREATE, PW:TYPE

<b>Arguments</b>	<"mtone_name"> ::= <string> is the name of the parametric multitone waveform. <ul style="list-style-type: none"> <li>• &lt;Hertz&gt; := &lt;NRf&gt; is the value of the frequency of the tone.</li> <li>• &lt;Volts&gt; := &lt;NRf&gt; is the value of the amplitude of the tone.</li> <li>• &lt;Gradients&gt; := &lt;NRf&gt; is the value of the phase of the tone.</li> <li>• MINimum sets or queries the minimum value of the parameter.</li> <li>• MAXimum sets or queries the maximum value of the parameter.</li> <li>• DEFault: sets the parameter to the default value.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:MULTit:ADD "My_Pwave_Mtone",10E6,0.5,50 Adds in 'My_Pwave_Mtone' parametric waveform a tone with 500 mV of amplitude, 10 Mhz of frequency and 50° of phase.

**Table 118: PW:MULTit:ADD**

<b>Command</b>	PW:MULTit:DELet (No Query Form)
<b>Description</b>	This command deletes a specific tone or all tones present in a parametric Multitone waveform.  <b>Note 1:</b> if the type of the parametric waveform is different from Multitone, this command reports an error. <b>Note 2:</b> if the index of the tone doesn't exist in the parametric multitone waveform, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:DELet <mtone_name>,{ ALL   < k > }
<b>Related Commands</b>	PW:CREATE, PW:TYPE, PW:MULTit:ADD
<b>Arguments</b>	<"mtone_name"> ::= <string> is the name of the parametric multitone waveform. <ul style="list-style-type: none"> <li>• k := &lt;NR1&gt; indicates the tone index. This value must be in the range 1 to 10.</li> <li>• ALL : deletes all tones from a parametric multitone waveform.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:MULTit:DELet "My_Pwave_Mtone",2 Deletes the second tone from 'My_Pwave_Mtone' parametric waveform.

**Table 119: PW:MULTit:DELet**

<b>Command</b>	PW:MULTit:TONe[k]:FREquency? (Query Only)
<b>Description</b>	<p>This command queries the frequency of a specified tone present in a parametric Multitone waveform.</p> <p><b>Note 1:</b> if the type of the parametric waveform is different from Multitone, this command reports an error.</p> <p><b>Note 2:</b> if the index of the tone doesn't exist in the parametric multitone waveform, this command reports an error.</p> <p><b>Note 3:</b> it is not possible to change the frequency of a single tone once it has already been created.</p>
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:TONe[k]:FREquency? <mtone_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPe, PW:MULTit:ADD
<b>Arguments</b>	<p>&lt;"mtone_name"&gt; ::= &lt;string&gt; is the name of the parametric multitone waveform.</p> <ul style="list-style-type: none"> <li>• k := &lt;NR1&gt; indicates the tone index. This value must be in the range 1 to 10.</li> <li>• MINimum sets or queries the minimum value of the parameter.</li> <li>• MAXimum sets or queries the maximum value of the parameter.</li> </ul>
<b>Returns</b>	<NRf>, value of frequency of a single tone
<b>Example</b>	PW:MULTit:TONe1:FREquency? "My_Pwave_Mtone" Might return 1.000E6.

**Table 120: PW:MULTit:TONe[k]:FREquency?**

<b>Command</b>	PW:MULTit:TONe[k]:AMPlitude
<b>Description</b>	<p>This command sets or queries the amplitude of a specified tone present in a parametric Multitone waveform.</p> <p><b>Note 1:</b> if the type of the parametric waveform is different from Multitone, this command reports an error.</p> <p><b>Note 2:</b> if the index of the tone doesn't exist in the parametric multitone waveform, this command reports an error.</p>

<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:TONe[k]:AMPlitude <mtone_name>,{MINimum   MAXimum   DEFault   <Volts>}, PW:MULTit:TONe[k]:AMPlitude? <mtone_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE, PW:MULTit:ADD
<b>Arguments</b>	<"mtone_name"> ::= <string> is the name of the parametric multitone waveform. <ul style="list-style-type: none"><li>• k := &lt;NR1&gt; indicates the tone index. This value must be in the range 1 to 10.</li><li>• MINimum sets or queries the minimum value of param.</li><li>• MAXimum sets or queries the maximum value of param.</li><li>• DEFault: sets the parameter to the default value.</li><li>• &lt;Volts&gt; := &lt;NRf&gt; is the value of the amplitude of the tone.</li></ul>
<b>Returns</b>	<NRf>
<b>Example</b>	PW:MULTit:TONe2:AMPlitude "My_Pwave_Mtone",0.6 Sets the amplitude of the second tone of 'My_Pwave_Mtone' parametric waveform to 600 mV.  PW:MULTit:TONe2:AMPlitude? "My_Pwave_Mtone" Might return 0.600.

**Table 121: PW:MULTit:TONe[k]:AMPlitude**

<b>Command</b>	PW:MULTit:TONe[k]:PHAsE
<b>Description</b>	This command sets or queries the phase of a specified tone present in a parametric Multitone waveform.  <b>Note 1:</b> if the type of the parametric waveform is different from Multitone, this command reports an error. <b>Note 2:</b> if the index of the tone doesn't exist in the parametric multitone waveform, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:TONe[k]:PHAsE <mtone_name>,{MINimum   MAXimum   DEFault   <Gradients>}, PW:MULTit:TONe[k]:PHAsE? <mtone_name>,[{MINimum   MAXimum}]
<b>Related Commands</b>	PW:CREATE, PW:TYPE,

	PW:MULTit:ADD
<b>Arguments</b>	<p>&lt;"mtone_name"&gt; ::= &lt;string&gt; is the name of the parametric multitone waveform.</p> <ul style="list-style-type: none"> <li>• k := &lt;NR1&gt; indicates the tone index. This value must be in the range 1 to 10.</li> <li>• MINimum sets or queries the minimum value of param.</li> <li>• MAXimum sets or queries the maximum value of param.</li> <li>• DEFault: sets the parameter to the default value.</li> <li>• &lt;Gradients&gt; := &lt;NRf&gt; is the value of the phase of the tone.</li> </ul>
<b>Returns</b>	<NRf>
<b>Example</b>	<pre>PW:MULTit:TOne3:PHAse "My_Pwave_Mtone",30 Sets the phase of the third tone of 'My_Pwave_Mtone' parametric waveform to 30°.</pre> <pre>PW:MULTit:TOne3:PHAse? "My_Pwave_Mtone" Might return 30.</pre>

**Table 122: PW:MULTit:TOne[k]:PHAse**

<b>Command</b>	PW:MULTit:NUM? (Query Only)
<b>Description</b>	This command queries the total number of tones present in a parametric Multitone waveform.  <b>Note:</b> if the type of the parametric waveform is different from Multitone, this command reports an error.
<b>Group</b>	Parametric Waveforms
<b>Syntax</b>	PW:MULTit:NUM? <mtone_name>
<b>Related Commands</b>	PW:CREATE, PW:TYPE, PW:MULTit:ADD
<b>Arguments</b>	<"mtone_name"> ::= <string> is the name of the parametric multitone waveform.
<b>Returns</b>	<NR1> := number of tones.
<b>Example</b>	<pre>PW:MULTit:NUM? "My_Pwave_Mtone" Might return 3.</pre>

**Table 123: PW:MULTit:NUM?**

## 6.10 MEMORY GROUP COMMANDS

<b>Command</b>	*RCL (No Query Form)
<b>Description</b>	This command restores the state of the instrument from a copy of the settings stored in a specified setup memory location. The settings are stored using the *SAV command.
<b>Group</b>	Memory
<b>Syntax</b>	*RCL {0 1 2 3 4}
<b>Related Commands</b>	*SAV
<b>Arguments</b>	0, 1, 2, 3, or 4: specifies the setup memory. Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration, location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration.
<b>Returns</b>	None
<b>Example</b>	*RCL 3 Restores the instrument from a copy of the settings stored in memory location 3.

**Table 124: \*RCL**

<b>Command</b>	*SAV (No Query Form)
<b>Description</b>	This command stores the current AWG settings to a specified setup memory location.  The current AWG configuration is automatically saved every time the user changes a parameter. This configuration, here named "current configuration" is automatically loaded at the power on.  Note: If a specified numbered setup memory is locked, this command causes an error.
<b>Group</b>	Memory
<b>Syntax</b>	*SAV {0 1 2 3 4}
<b>Related Commands</b>	*RCL
<b>Arguments</b>	0, 1, 2, 3, or 4: specifies the setup memory. Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration,

	location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration.
<b>Returns</b>	None
<b>Example</b>	*SAV 2 Saves the current instrument state in the memory location 2.

**Table 125: \*SAV**

<b>Command</b>	MEMORY:NStates? (Query Only)
<b>Description</b>	This command returns the total number of available configurations saved in the Configuration List memory.
<b>Group</b>	Memory
<b>Syntax</b>	MEMORY:NStates?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value
<b>Example</b>	MEMORY:NStates? Might return 2.

**Table 126: MEMORY:NStates**

<b>Command</b>	MEMORY:STATE:CATalog? (Query Only)
<b>Description</b>	This command lists the names of available configurations saved in the Configuration List memory.
<b>Group</b>	Memory
<b>Syntax</b>	MEMORY:STATE:CATalog?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<cfg_name>[,<cfg_name>[,<cfg_name>[,<cfg_name>]]] <cfg_name> ::= <string>
<b>Example</b>	MEMORY:STATE:CATalog? Might return My_Configuration, Configuration_20190110_183606_568, Test1, MEM_1.

**Table 127: MEMORY:STATE:CATalog**

<b>Command</b>	MEMORY:STATE:DElete (No Query Form)
<b>Description</b>	This command deletes the specified configuration. If the specified configuration is locked or not present this command causes an error.

<b>Group</b>	Memory
<b>Syntax</b>	MEMORY:STATE:DElete {0 1 2 3 4 <cfg_name>}
<b>Related Commands</b>	None
<b>Arguments</b>	0, 1, 2, 3, 4 or <cfg_name> where: <cfg_name> ::= <string> specifies the configuration. 0, 1, 2, 3, or 4: specifies the setup memory. Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration, location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration.
<b>Returns</b>	None
<b>Example</b>	MEMORY:STATE:DElete 1 Deletes the configuration "MEM_1".

**Table 128: MEMORY:STATE:DElete**

<b>Command</b>	MEMORY:STATE:LOCK
<b>Description</b>	This command sets or queries whether to lock the specified configuration. If you lock a configuration, you cannot overwrite or delete the setup file.
<b>Group</b>	Memory
<b>Syntax</b>	MEMORY:STATE:LOCK {0 1 2 3 4 <cfg_name>},{OFF ON} MEMORY:STATE:LOCK? {0 1 2 3 4 <cfg_name>}
<b>Related Commands</b>	None
<b>Arguments</b>	0, 1, 2, 3, 4, <cfg_name>, where: <cfg_name> ::= <string> specifies the configuration to locked or queried. 0, 1, 2, 3, or 4: specifies the setup memory. Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration, location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration. ON or <NR1>#0 locks the specified configuration. OFF or <NR1>=0 allows you to overwrite or delete the specified configuration.
<b>Returns</b>	A single <NR1>
<b>Example</b>	MEMORY:STATE:LOCK 1,ON Locks the configuration "MEM_1"

**Table 129: MEMORY:STATE:LOCK**

<b>Command</b>	MEMory:STATe:NAME
<b>Description</b>	This command copies a configuration with "src_name" in "dst_name" configuration. If a configuration with "dst_name" is already present an error will occur. The query command returns the names referred to the location 0, 1, 2, 3, 4. The names will be ever the same: "MEM_0", "MEM_1", "MEM_2", "MEM_3", "MEM_4".
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:STATe:NAME {0 1 2 3 4 <src_cfg_name>},{0 1 2 3 4 <dst_cfg_name>} MEMory:STATe:NAME? {0 1 2 3 4}
<b>Related Commands</b>	None
<b>Arguments</b>	0, 1, 2, 3, 4, <src_cfg_name>, <dst_cfg_name> where: <src_cfg_name> ::= <string> specifies the source configuration name. <dst_cfg_name> specifies the destination configuration name. 0, 1, 2, 3, or 4: specifies the setup memory. Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration, location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration.
<b>Returns</b>	<cfg_name> where <cfg_name> ::= <string>
<b>Example</b>	MEMory:STATe:NAME 1,"TEST_RACK_1" Copies configuration "MEM_1" in configuration "TEST_RACK_1". MEMory:STATe:NAME? 2 Might return MEM_2.

**Table 130: MEMory:STATe:NAME**

<b>Command</b>	MEMory:STATe:VALid? (Query Only)
<b>Description</b>	This command returns the availability of a configuration.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:STATe:VALid? {0 1 2 3 4 <src_cfg_name>}
<b>Related Commands</b>	None
<b>Arguments</b>	0, 1, 2, 3, 4, <scfg_name> where: <src_cfg_name> ::= <string> specifies the configuration name. 0, 1, 2, 3, or 4: specifies the setup memory.

	Location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration, location 2 refers to "MEM_2" configuration, location 3 refers to "MEM_3" configuration and location 4 refers to "MEM_4" configuration.
<b>Returns</b>	<NR1> 1 means that the specified configuration is present in Saved configuration list. 0 means that the specified configuration is not present.
<b>Example</b>	MEMORY:STATE:VALID? 0 Might return 1 if the specified setup memory has been saved.

**Table 131: MEMORY:STATE:VALID?**

<b>Command</b>	DElete:SETUp (No Query Form)
<b>Description</b>	This command deletes a configuration.
<b>Group</b>	Memory
<b>Syntax</b>	DElete:SETUp <cfg_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<cfg_name>::=<string>
<b>Returns</b>	None
<b>Example</b>	DElete:SETUp “test” Deletes the configuration named test.

**Table 132: DElete:SETUp**

<b>Command</b>	RECALL:SETUp (No Query Form)
<b>Description</b>	This command recalls a configuration. This command is equivalent to AWGControl:SREStore.
<b>Group</b>	Memory
<b>Syntax</b>	RECALL:SETUp <cfg_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<cfg_name>::=<string> specifies the configuration.
<b>Returns</b>	None
<b>Example</b>	RECALL:SETUp “test” Restores the instrument configuration named “test”.

**Table 133: RECALL:SETUp**

## 6.11 MASS MEMORY GROUP COMMANDS

<b>Command</b>	MMEMemory:CATalog? (Query only)
<b>Description</b>	<p>This command returns a list of information concerning the contents of the current directory of the file system on the AWG. In particular it returns the list of all files and directories present there specifying their names and sizes. It reports also the dimension of free space of the mass storage in bytes.</p> <p><b>NOTE:</b> By default "C:\Users\awg3000\Pictures\Saved Pictures" is the current directory of the file system.</p> <p><b>NOTE:</b> In the description of the remaining commands, the 'awg3000' folder will be replaced by &lt;username&gt; folder.</p> <p><b>NOTE:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMemory commands; it's subdirectories can be accessed via the MMEMemory:CDIRectory command.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMemory:CATalog[:ALL]?
<b>Related Commands</b>	MMEMemory:CDIRectory MMEMemory:MSIS
<b>Arguments</b>	None
<b>Returns</b>	<p>&lt;NR1&gt;,&lt;file_entry&gt;,&lt;file_entry&gt;,&lt;file_entry&gt;,..... where:  &lt;NR1&gt; indicates the free space of the mass storage in bytes,  &lt;file_entry&gt; ::= "&lt;file_name&gt;,&lt;file_type&gt;,&lt;file_size&gt;" where:  &lt;file_name&gt; ::= &lt;string&gt; is the exact name of the file,  &lt;file_type&gt; ::= is DIR for an entry that is a directory, empty/blank otherwise,  &lt;file_size&gt; ::= &lt;NR1&gt; is the size of the file in bytes. For &lt;file_type&gt; marked DIR, the file size will always be 0.</p>
<b>Example</b>	<pre>MMEMemory:CATalog? It might return: 3878652,"SAMPLE1.ZIP,,2948","aaa.txt,,1024","MY_WAVES,DIR,0"</pre>

Table 134: MMEMemory:CATalog?

<b>Command</b>	MMEMemory:CDIRectory
<b>Description</b>	This command sets or returns the current directory of the file system on the AWG. This command is strictly related to MMEMemory:MSIS

	<p>command that permits to set the mass storage unit &lt;msus&gt; namely the unit used by all MMEMory commands.</p> <p>The current directory for the programmatic interface is different from the currently selected directory in the Windows Explorer on the AWG.</p> <p><b>NOTE:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:CDIRectory [<directory_name>] MMEMory:CDIRectory?
<b>Related Commands</b>	None
<b>Arguments</b>	<directory_name> ::= <string>
<b>Returns</b>	<directory_name>
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MMEMORY:CDIRECTORY "configurations" Changes the current directory to "C:\Users\&lt;username&gt;\Pictures\Saved Pictures\configurations".</p> <p>Assuming the current &lt;msus&gt; is "D:" MMEMORY:CDIRECTORY "tmp" Changes the current directory to "D:\tmp"</p> <p>MMEMORY:CDIRECTORY? Might return "Users\&lt;username&gt;\Pictures\Saved Pictures\configurations".</p>

**Table 135: MMEMory:CDIRectory**

<b>Command</b>	MMEMory:COPY (No Query Form)
<b>Description</b>	<p>This command copies &lt;source_file&gt; into &lt;target_file&gt;. The file names must include any file extension.</p> <p>If target_file already exists it will be overwritten.</p> <p><b>NOTE 1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands.</p>

	<b>NOTE 2:</b> Only files with the following extension can be copied: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:COPY <source_file>,<target_file>
<b>Related Commands</b>	None
<b>Arguments</b>	<p>&lt;source_file&gt; ::= &lt;string&gt;  &lt;target_file&gt; ::= &lt;string&gt;</p> <p>Both of them could be absolute or relative (respect current directory) paths.</p>
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MMMEMORY:COPY "source.txt","D:\My_Waves\target.txt"</p> <p>Copies "source.txt" located in "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory in "target.txt" located in "D:\My_Waves" directory .</p>

**Table 136: MMEMORY:COPY**

<b>Command</b>	MMEMORY:DATA
<b>Description</b>	<p>This command sets or returns block data to/from a file in the current mass storage device.</p> <p>The file path may contain a full file path. However, if the file path only contains a file name, the current directory is assumed.</p> <p><b>NOTE 1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands.</p> <p><b>NOTE 2:</b> Only files with the following extension can be manipulated: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:DATA <file_name>,<start_index>,<block_data> MMEMORY:DATA? <file_name>[,<start_index>[,<size>]]
<b>Related Commands</b>	MMEMORY:CDIRectory, MMEMORY:MSIS
<b>Arguments</b>	<file_name> ::= <string> could be absolute or relative path.

	<p>&lt;start_index&gt; ::= &lt;NR1&gt; is the index of byte of the desired &lt;file_name&gt; where writing/reading operations will start.</p> <p>&lt;size&gt; ::= &lt;NR1&gt; is the size, in bytes, to write/read.</p> <p>&lt;block_data&gt; ::= see Block Data Format chapter (IEEE 488.2 data block).</p>
<b>Returns</b>	<block_data> ::= IEEE 488.2 block data format.
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MMEMORY:DATA "123.TXT",#13ABC Loads "ABC" into 123.TXT in the current directory.</p> <p>MMEMORY:DATA "data.txt",1024,#2048XXXXXX... Inserts 2048 bytes specified by XXXXXX... values of in file "data.txt" in the current directory.</p> <p>MMEMORY:DATA? "D:\tmp\waveform.txt",2048,1024 Returns #41024XXXX.... where XXXX.... are 1024 bytes of file "waveform.txt" located in "D:\tmp" starting from 2048-th byte.</p>

**Table 137: MMEMORY:DATA**

<b>Command</b>	MMEMORY:DATA:SIZE? (Query Only)
<b>Description</b>	<p>This command returns the size in bytes of a selected file.</p> <p><b>NOTE 1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands.</p> <p><b>NOTE 2:</b> Only files with the following extension can be manipulated: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:DATA:SIZE? <file_name>
<b>Related Commands</b>	MMEMORY:CDIRectory, MMEMORY:MSIS
<b>Arguments</b>	<file_name> ::= <string> it could be absolute or relative path.
<b>Returns</b>	<NR1> is the size, in bytes, of the selected file
<b>Example</b>	Assuming the current <msus> is "C:" and current directory "C:\Users\<username>\Pictures\Saved Pictures".

	<pre>MMEMORY:DATA:SIZE? "data.bin" Might return 1024. MMEMORY:DATA:SIZE? "D:\tmp\waveform.txt" Might return 65535.</pre>
--	--

**Table 138: MMEMORY:DATA:SIZE?**

<b>Command</b>	MMEMORY:DELETE (No Query Form)
<b>Description</b>	<p>This command deletes a file or directory from the AWG's accessible files system.</p> <p><b>NOTE 1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands.</p> <p><b>NOTE 2:</b> Only files with the following extension can be deleted: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:DELETE <file_name>[,<msus>]
<b>Related Commands</b>	MMEMORY:CDIRectory, MMEMORY:MSIS
<b>Arguments</b>	<file_name> ::= <string> could be absolute or relative path. <msus> (mass storage unit specifier) ::= <string>
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <pre>MMEMORY:DELETE "data.bin" Deletes "data.bin" from the current directory.</pre> <pre>MMEMORY:DELETE "\my\proj\awg\test.txt","D:" Deletes "test.txt" from "D:\my\proj\awg" directory.</pre>

**Table 139: MMEMORY:DELETE**

<b>Command</b>	MMEMORY:DOWNload:DATA (No Query Form)
<b>Description</b>	<p>This command downloads data from the host computer to a file in the instrument. The filename must have been previously specified by MMEMORY:DOWNload:FNAME.</p>

	<p>The data in &lt;binary_block&gt; is written to the select file, and any data previously stored in the file is lost.</p> <p><b>NOTE:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands.</p>
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMory:DOWNload:DATA <binary_block>
<b>Related Commands</b>	MMEMory:DOWNload:FNAMe
<b>Arguments</b>	Any IEEE-488 definite or indefinite block
<b>Returns</b>	None
<b>Example</b>	<p>Writes the word "Hello" to the file "D:\Myfile.txt" on internal storage.</p> <p>MMEM:DOWN:FNAM "D:\Myfile.txt"</p> <p>MMEM:DOWN:DATA #15Hello</p>

**Table 140: MMEMory:DOWNload:DATA**

<b>Command</b>	MMEMory:DOWNload:FNAMe (No Query Form)
<b>Description</b>	<p>This command creates or opens the specified filename prior to writing data to that file with MMEMory:DOWNload:DATA.</p> <p><b>NOTE:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands.</p>
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMory:DOWNload:FNAMe <filename>
<b>Related Commands</b>	MMEMory:DOWNload:DATA
<b>Arguments</b>	Any valid file name
<b>Returns</b>	None
<b>Example</b>	<p>Writes the word "Hello" to the file "D:\Myfile.txt" on the internal flash file system.</p> <p>MMEM:DOWN:FNAM "D:\Myfile.txt"</p> <p>MMEM:DOWN:DATA #15Hello</p>

**Table 141: MMEMory:DOWNload:FNAMe**

<b>Command</b>	MMEMory:EXPort (No Query Form)
<b>Description</b>	This command exports a waveform from the current waveform list to an archive file (.zip).

	<p><b>NOTE 1</b> .zip is a zip file with property format.</p> <p><b>NOTE 2:</b> It's not possible export a predefined waveform from waveform list.</p> <p><b>NOTE 3:</b> If the archive file name is already present in the destination directory, the file will be overwritten.</p> <p><b>NOTE4:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands. The archive path may contain a full file path. However, if the file path only contains an archive name, the archive waveform will be exported starting from the current directory.</p> <p><b>NOTE 5:</b> This operation is the same as that it can be done through the software menu: Wave. List -&gt; Export.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:EXPort <wfm_name>,<archive_name>
<b>Related Commands</b>	None.
<b>Arguments</b>	<wfm_name>::=<string> is a name in waveform list, <archive_name>::=<string>.zip could be absolute or relative path. The extension .zip must always be specified in archive name.
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MMEMORY:EXPORT "sine1024","d:\waveforms\arc.zip"</p> <p>Exports a waveform named "sine1024" into "d:\waveform\arc.zip" file.</p>

**Table 142: MMEMory:EXPort**

<b>Command</b>	MMEMory:IMPort (No Query Form)
<b>Description</b>	This command imports a file into the current configuration waveforms list.
	<p><b>NOTE 1:</b> It's possible import a file only with the following extensions: .txt, .trc, .bin and .zip - property format-.</p>

	<p><b>NOTE 2:</b> If a .zip file is imported, the parameter {ANALog   DIGitals} will be not taken into consideration. The .zip format already contains this information.</p> <p><b>NOTE 3:</b> If the waveform name (wfm_name) has already present in waveform list, an error will be occurred.</p> <p><b>NOTE 4:</b> If waveform type {ANALog   DIGitals} isn't specify, ANALog type will be assumed as default.</p> <p><b>NOTE 5:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands. The file path may contain a full file path. However, if the file path only contains a file name, the current directory is assumed as destination directory.</p> <p><b>NOTE 6:</b> This operation is the same as that it can be done through the software menu: Wave. List -&gt; Import.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:IMPort <wfm_name>,<archive_name>[,{ANALog   DIGitals}]
<b>Related Commands</b>	MMEMory:OPEN
<b>Arguments</b>	<wfm_name>::=<string>, <archive_name> ::=<string>.{zip   trc   txt   bin} could be absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\ Pictures\Saved Pictures".</p> <p>MMEMORY:IMPORT "Test1","D:\TestFiles\waveform1.zip" Imports waveform1.zip file in waveform Test1 of waveform list (its type is already specified in .zip file).</p> <p>MMEMORY:IMPORT "Test2"," waveform2.txt",DIG Imports waveform2.txt file in waveform Test2 of waveform list (its type will be digital).</p>

**Table 143: MMEMory:IMPort**

<b>Command</b>	MMEMemory:LOAD:ALL (No Query Form)
<b>Description</b>	<p>This command uploads a complete configuration present in an archive (.zip) and applies it in place of the current configuration. This operation is performed in two steps:</p> <ol style="list-style-type: none"> <li>1. First the archive is loaded into the configurations list. Note: <ul style="list-style-type: none"> <li>• The name of the archive file is used as the name of the imported configuration (my_configuration.zip =&gt; my_configuration).</li> <li>• If a configuration with the same name is already present, the configuration is replaced.</li> <li>• If a configuration with the same name is already present and is located then an error occurs.</li> <li>• This operation is the same as that it can be done through the software menu: More -&gt; Load From -&gt; Import.</li> </ul> </li> <li>2. Once the archive has been imported into the configuration list, the new configuration will be loaded as current configuration.</li> </ol> <p><b>NOTE 1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMemory commands. The archive path may contain a full file path. However, if the file path only contains an archive name, the archive will be searched starting from the current directory.</p> <p><b>NOTE 2:</b> When this command is executed the AWG must be in idle state.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMemory:LOAD:ALL <archive_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<archive_name> ::= <string>.zip specifies a configuration file to be loaded. It could be absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MME:LOAD:ALL "configurations\my_configuration.zip"      Loads a complete instrument setup from the file      "my_configuration.zip" located in      "C:\Users\&lt;username&gt;\Pictures\Saved Pictures\configurations" directory.</p>

**Table 144: MMEMORY:LOAD:ALL**

<b>Command</b>	MMEMORY:LOAD:STATE (No Query Form)
<b>Description</b>	<p>This command imports a configuration saved in an archive (.zip) into the configurations list with the specified name.</p> <p><b>NOTE 1:</b> If a configuration with the same name is already present in configuration list then it will be replaced.</p> <p><b>NOTE 2:</b> If a configuration with the same name is already present in configuration list and it's locked then an error will occur.</p> <p><b>NOTE 3:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands. The archive path may contain a full file path. However, if the file path only contains an archive name, the archive will be searched starting from the current directory.</p> <p><b>NOTE 4:</b> This operation is equivalent to what the user can do through the following user interface menu: Other -&gt; Load from -&gt; Import</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:LOAD:STATE <archive_name>,{0 1 2 3 4}<cfg_name>
<b>Related Commands</b>	MEMORY:STATE:LOCK, MMEMORY:STORe:STATE
<b>Arguments</b>	<p>&lt;archive_name&gt;::=&lt;string&gt;.zip specifies a configuration file to be loaded. It could be absolute or relative path.</p> <p>It possible specify the configuration like:</p> <ul style="list-style-type: none"> <li>- 0 1 2 3 4: location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration...</li> <li>- &lt;cfg_name&gt;::=&lt;string&gt;: specifies the configuration name where will be saved the loaded configuration.</li> </ul>
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <pre>MMEMORY:LOAD:STATE "SETUP1.zip",1</pre>

	Loads the configuration file "SETUP1.zip" located in the current directory in "MEM_1".
--	--

**Table 145: MMEMORY:LOAD:STATE**

<b>Command</b>	MMEMORY:MDIRECTORY (No Query Form)
<b>Description</b>	<p>This command creates a new directory in the current path on the mass storage system.</p> <p><b>NOTE:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands.</p>
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMORY:MDIRECTORY <directory_name>
<b>Related Commands</b>	MMEMORY:CDIRECTORY, MMEMORY:MSIS
<b>Arguments</b>	<directory_name> ::= <string>
<b>Returns</b>	None
<b>Example</b>	<pre>MMEMORY:MDIRECTORY "Waveform" Creates the directory "Waveform" in the current directory.</pre>

**Table 146: MMEMORY:LOAD:STATE**

<b>Command</b>	MMEMORY:MOVE (No Query Form)
<b>Description</b>	<p>Moves &lt;file1&gt; to &lt;file2&gt;. The file names must include the file extension.</p> <p>The file path may contain a full file path. However, if the file path only contains a file name, the file will be searched starting from the current directory.</p> <p>If &lt;file2&gt; already exists it will be overwritten.</p> <p><b>NOTE1:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands.</p> <p><b>NOTE 2:</b> Only files with the following extension can be moved: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.</p>
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMORY:MOVE <file1>,<file2>
<b>Related Commands</b>	None

<b>Arguments</b>	<file1>,<file2> they could be absolute or relative paths.
<b>Returns</b>	None
<b>Example</b>	MMEM:MOVE "MySetup.zip","D:\Backup.zip" MMEM:MOVE "D:\arbMonday.txt", "D:\arbTuesday.bin"

**Table 147: MMEMory:LOAD:STATe**

<b>Command</b>	MMEMory:MSIS
<b>Description</b>	<p>This command selects or returns a mass storage device used by all MMEMory commands. &lt;msus&gt; specifies a drive using a drive letter. The drive letter can represent hard disk drives or external USB storage memory.</p> <p><b>NOTE 1:</b> Every time the &lt;msus&gt; changes the current directory is reset to the root folder.</p> <p><b>NOTE 2:</b> If the new &lt;msus&gt; is the "C:" unit, the current directory is reset to "C:\Users\awg3000\Pictures\Saved Pictures" folder.</p>
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMory:MSIS [<msus>] MMEMory:MSIS?
<b>Related Commands</b>	None
<b>Arguments</b>	<msus> (mass storage unit specifier)::= <string>
<b>Returns</b>	<p>&lt;msus&gt;</p> <p>NOTE. If the mass storage device has not been defined, the returned &lt;msus&gt; value is the system's default drive which is typically the :C drive.</p>
<b>Example</b>	<p>MMEMORY:MSIS "D:"</p> <p>Changes the MSUS to the D: drive where D: is a USB memory.</p> <p>MMEMORY:MSIS?</p> <p>Might return "E:", assuming the current MSUS is the E: drive.</p>

**Table 148:MMEMory:MSIS**

<b>Command</b>	MMEMory:OPEN (No Query Form)
<b>Description</b>	This command imports a waveform stored in a file (.zip, .txt, .trc, .bin) into the waveform list of the current AWG's.

	<p><b>NOTE 1:</b> If waveform file has ".zip" extension then the parameter {ANALog   DIGItals} will not be taken into account. The ".zip" format already has this information in itself.</p> <p><b>NOTE 2:</b> The waveform name will be derived directly from the archive name.</p> <p><b>NOTE 3:</b> If the waveform name is already present in the waveform list then an error will occur.</p> <p><b>NOTE 4:</b> If the waveform type {ANALog   DIGItals} is not specified, the ANALog type will be assumed as default.</p> <p><b>NOTE 5:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMory commands. The waveform path may contain a full file path. However, if the file path only contains a waveform name, the waveform will be searched starting from the current directory.</p> <p><b>NOTE 6:</b> This operation is equivalent to what the user can do through the following user interface menu: Wave. List -&gt; Import</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:OPEN <filepath>[,{ANALog   DIGItals}]
<b>Related Commands</b>	None
<b>Arguments</b>	<filepath> ::= <string>.{zip   txt   trc   bin} could be an absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p>MMEMORY:OPEN "D:\TestFiles\WFM_001.txt",DIG</p> <p>After command execution, if no errors occur, digital waveform WFM_001 will appear into the AWG's waveform list. WFM_001 was originally located in "D:\TestFiles" directory.</p>

**Table 149: MMEMory:OPEN**

<b>Command</b>	MMEMory:OPEN:SETup (No Query Form)
----------------	------------------------------------

<b>Description</b>	This command uploads a complete configuration present in an archive (.zip) and applies it in place of the current configuration.  <b>NOTE 1:</b> It's an alias of MMEMORY:LOAD:ALL command. See its description for more informations. <b>NOTE 2:</b> The AWG must be in idle state.
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:OPEN:SETup <filepath>
<b>Related Commands</b>	None
<b>Arguments</b>	<filepath> ::= <string>.zip could be an absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	MMEMORY:OPEN:SETUP "D:\TestFiles\mySetup.zip" Opens and applies the setup file mySetup.zip.

**Table 150: MMEMORY:OPEN:SETup**

<b>Command</b>	MMEMORY:RDIRectory (No Query Form)
<b>Description</b>	This command removes an empty directory (folder) from the mass storage system.  <b>NOTE:</b> Only removable units and "C:\Users\<username>\Pictures\Saved Pictures" directory are accessible by MMEMORY commands. The directory path may contain a full path. However, if only directory name is specified, the directory will be searched starting from the current directory.
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMORY:RDIRectory <folder>
<b>Related Commands</b>	None
<b>Arguments</b>	<folder>::=<string> could be an absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	If the current directory is "C:\Users\<username>\Pictures\Saved Pictures"  MMEMORY:RDIRectory "Test" Removes the empty folder "Test" from the current directory.

**Table 151:MMEMORY:RDIRectory**

<b>Command</b>	MMEMORY:STORe:ALL (No Query Form)
----------------	-----------------------------------

<b>Description</b>	This command saves the current AWG's configuration in an archive (.zip).  <b>NOTE 1:</b> If an archive with the same name and path is already present then the archive is overwritten.  <b>NOTE 2:</b> Only removable units and "C:\Users\<username>\Pictures\Saved Pictures" directory are accessible by MMEMory commands. The archive path may contain a full path. However, if only name is specified, the archive will be saved starting from the current directory.
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:STORe:ALL <filename>
<b>Related Commands</b>	None
<b>Arguments</b>	<filename> ::= <string>.zip could be an absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	Assuming the current <msus> is "C:" and current directory "C:\Users\<username>\Pictures\Saved Pictures".  MMEMory:STORe:ALL "D:\mySetup.zip" Saves the current instrument's configuration in mySetup.zip file in drive D:.

**Table 152: MMEMory:STORe:ALL**

<b>Command</b>	MMEMory:SAVE:SETup (No Query Form)
<b>Description</b>	This command saves the current AWG's configuration in an archive (.zip).  <b>NOTE 1:</b> It's an alias of MMEMory:STORe:ALL command. See its description for more informations.
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:SAVE:SETup <filename>
<b>Related Commands</b>	None
<b>Arguments</b>	<filename> ::= <string>.zip could be an absolute or relative path.
<b>Returns</b>	None
<b>Example</b>	Assuming the current <msus> is "C:" and current directory "C:\Users\<username>\Pictures\Saved Pictures".

	MMEMORY:SAVE:SETUP " mySetup.zip" Saves the current instrument's configuration in "C:\Users\<username>\Pictures\Saved Pictures\mySetup.zip " file.
--	--

**Table 153: MMEMORY:SAVE:SETUP**

<b>Command</b>	MMEMORY:STORe:STATe (No Query Form)
<b>Description</b>	<p>This command saves a configuration present in the configurations list in an archive (.zip).</p> <p><b>NOTE 1:</b> If an archive with the same path and name is already present then it will be overwritten.</p> <p><b>NOTE 2:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by MMEMORY commands. The archive path may contain a full path. However, if only name is specified, the archive will be saved starting from the current directory.</p>
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMORY:STORe:STATe {0 1 2 3 4 <cfg_name>}, <archive_name>
<b>Related Commands</b>	MMEMORY:LOAD:STATe, MMEMORY:LOCK[:STATe]
<b>Arguments</b>	<p>It possible specify the configuration like:</p> <ul style="list-style-type: none"> <li>- 0 1 2 3 4: location 0 refers to "MEM_0" configuration, location 1 refers to "MEM_1" configuration...</li> <li>- &lt;cfg_name&gt;::=&lt;string&gt;</li> </ul> <p>&lt;archive_name&gt;::=&lt;string&gt;.zip specifies the file path. It could be an absolute or relative path.</p>
<b>Returns</b>	None
<b>Example</b>	<p>Assuming the current &lt;msus&gt; is "C:" and current directory "C:\Users\&lt;username&gt;\Pictures\Saved Pictures".</p> <p><b>MMEMORY:STORE:STATE 1,"setup1.zip"</b> Copies the configuration stored in the setup memory location 1 to a file named "setup1.zip" in the current directory.</p>

**Table 154: MMEMORY:STORe:STATe**

<b>Command</b>	MMEMORY:UPLoad? (Query Only)
----------------	------------------------------

<b>Description</b>	This command returns the contents of a file.  <b>NOTE 1:</b> Only removable units and "C:\Users\<username>\Pictures\Saved Pictures" directory are accessible by MMEMory commands.  <b>NOTE 2:</b> Only files with the following extension can be deleted on removable units: .jpeg, .png, .bmp, .jpg, .gif, .tiff, .zip, .txt, .trc, .bin.
<b>Group</b>	Mass memory
<b>Syntax</b>	MMEMory:UPLoad? <file_name>
<b>Related Commands</b>	MMEMory:CDIRectory, MMEMory:MSIS
<b>Arguments</b>	<file_name> ::= <string> could be absolute or relative paths.
<b>Returns</b>	<block_data> ::= IEEE 488.2 block data format
<b>Example</b>	MMEM:UPL? "D:\Myfile.zip" Returns the contents of "Myfile.zip".

**Table 155: MMEMory:UPLoad?**

## 6.12 STATUS GROUP COMMANDS

<b>Command</b>	STATUs:OPERation:CONDition? (Query Only)
<b>Description</b>	This query returns the contents of the Operation Condition Register.
<b>Group</b>	Status
<b>Syntax</b>	STATUs:OPERation:CONDition?
<b>Related Commands</b>	STATUs:OPERation:ENABLE, STATUs:OPERation[:EVENT]?
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value showing the contents of the OCR.
<b>Example</b>	<p>STATUs:OPERation:CONDition?</p> <p>Might return 8, showing that the bits in the OCR have the binary value 000000000001000 that indicates that the instrument is waiting for a trigger event to occur.</p>

**Table 156: STATUs:OPERation:CONDition?**

<b>Command</b>	STATUs:OPERation:ENABLE
<b>Description</b>	This command sets or returns the mask for the Operation Enable Register (OENR). Note that the OENR is not used.
<b>Group</b>	Status
<b>Syntax</b>	STATUs:OPERation:ENABLE <enable_value> STATUs:OPERation:ENABLE?
<b>Related Commands</b>	None
<b>Arguments</b>	<enable_value> ::= <NR1> is the enable mask of the OENR. Range: 0 to 65535.
<b>Returns</b>	<enable_value>
<b>Example</b>	<p>STATUs:OPERation:ENABLE?</p> <p>Might returns 0.</p>

**Table 157: STATUs:OPERation:ENABLE**

<b>Command</b>	STATUs:OPERation[:EVENT]? (Query Only)
<b>Description</b>	This command returns the value (in decimal) sets in the Operation Event Register (OEVR) and clears the OEVR. OEVR is a transition register for OCR. This command is query only.
<b>Group</b>	Status
<b>Syntax</b>	STATUs:OPERation[:EVENT]?
<b>Related Commands</b>	STATUs:OPERation:CONDition?, STATUs:OPERation:ENABLE
<b>Arguments</b>	None

<b>Returns</b>	A single <NR1> value showing the contents of the OEVR.
<b>Example</b>	<p>STATus:OPERation:EVENT?</p> <p>Might return 8, which indicates that the OEVR contains the binary number 00000001000; it means that the status of Bit_3 of OCR register has changed.</p>

**Table 158: STATus:OPERation[:EVENT]?**

<b>Command</b>	STATus:PRESet (No Query Form)
<b>Description</b>	This command sets the Operation Enable Register (OENR) and Questionable Enable Register (QENR). Both registers are not used.
<b>Group</b>	Status
<b>Syntax</b>	STATus:PRESet
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	<p>STATUS:PRESET</p> <p>Resets the SCPI enable registers (not used).</p>

**Table 159: STATus:PRESet**

<b>Command</b>	STATus:QUESTIONable:CONDITION? (Query Only)
<b>Description</b>	This query returns the status of the Questionable Condition Register. Not used in this version.
<b>Group</b>	Status
<b>Syntax</b>	STATus:QUESTIONable:CONDITION?
<b>Related Commands</b>	<p>STATus:QUESTIONable:ENABLE?</p> <p>STATus:QUESTIONable[:EVENT]?</p>
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	<p>STATUS:QUESTIONABLE:CONDITION?</p> <p>Allways returns 0.</p>

**Table 160: STATus:QUESTIONable:CONDITION?**

<b>Command</b>	STATus:QUESTIONable:ENABLE
<b>Description</b>	This command sets or returns the enable mask of the Questionable Enable Register (QENR) which allows true conditions in the Questionable Event Register to be reported in the summary bit. Not used in this version.

<b>Group</b>	Status
<b>Syntax</b>	STATUs:QUESTIONable:ENABLE <enable_value> STATUs:QUESTIONable:ENABLE?
<b>Related Commands</b>	STATUs:QUESTIONable:CONDITION?, STATUs:QUESTIONable[:EVENT]?
<b>Arguments</b>	<enable_value> ::= <NR1> is the enable mask of the QENR. Range: 0 to 65535.
<b>Returns</b>	A single <NR1> value showing the contents of the QENR.
<b>Example</b>	STATUs:QUESTIONable:ENABLE? Might return 0.

**Table 161: STATUs:QUESTIONable:ENABLE**

<b>Command</b>	STATUs:QUESTIONable[:EVENT]? (Query Only)
<b>Description</b>	This command returns the contents of the Questionable Event Register (QEVR). Reading the QEVR clears it. Not used in this version.
<b>Group</b>	Status
<b>Syntax</b>	STATUs:QUESTIONable[:EVENT]?
<b>Related Commands</b>	STATUs:QUESTIONable:CONDITION?, STATUs:QUESTIONable:ENABLE
<b>Arguments</b>	None
<b>Returns</b>	0
<b>Example</b>	STATUs:QUESTIONable: EVENT? Always returns 0.

**Table 162: STATUs:QUESTIONable[:EVENT]?**

<b>Command</b>	*STB? (Query Only)
<b>Description</b>	This query returns the contents of Status Byte Register.
<b>Group</b>	Status
<b>Syntax</b>	*STB?
<b>Related Commands</b>	*CLS, *ESE, *ESR?, *SRE
<b>Arguments</b>	None
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	*STB? Might return 96, which indicates that the SBR contains the binary number 0110 0000.

**Table 163: \*STB?**

<b>Command</b>	*PSC
----------------	------

<b>Description</b>	This command sets and queries the power-on status flag that controls the automatic power-on execution of SRER and ESER. When *PSC is true, SRER and ESER are set to 0 at power-on. When *PSC is false, the current values in the SRER and ESER are preserved in nonvolatile memory when power is shut off and are restored at power-on.
<b>Group</b>	Status
<b>Syntax</b>	*PSC {0   1} *PSC?
<b>Related Commands</b>	None
<b>Arguments</b>	<p>&lt;NR1&gt;=0            Sets the power-on status clear flag to false, disables the power-on clear, and allows the instrument to possibly assert SRQ after power-on.</p> <p>&lt;NR1&gt;#0            Sets the power-on status clear flag true; sending *PSC 1 therefore enables the power-on status clear and prevents any SRQ assertion after power-on</p>
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	PSC 0 Sets the power-on status clear flag to false.

**Table 164: \*PSC**

## 6.13 SYSTEM GROUP COMMANDS

<b>Command</b>	SYSTem:BEEPer:STATE
<b>Description</b>	The SYSTem:BEEPer:STATE command sets the beeper ON or OFF. The SYSTem:BEEPer:STATE? command returns "0" (OFF) or "1" (ON). When the beeper is set to ON, the instrument will beep when an error message or a warning message is displayed on the screen. The instrument does not beep when an error or warning caused by remote command execution.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:BEEPer:STATE {OFF   ON} SYSTem:BEEPer:STATE?
<b>Related Commands</b>	None
<b>Arguments</b>	ON or <NR1>#0 Enables the beeper OFF or <NR1>=0 Disables the beeper
<b>Returns</b>	A single <NR1> value.
<b>Example</b>	SYSTem:BEEPer:STATE ON Enables the beeper function

Table 165: SYSTem:BEEPer:STATE

<b>Command</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Description</b>	This command causes the instrument to beep immediately.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Related Commands</b>	None
<b>Arguments</b>	ON or <NR1>#0 Enables the beeper OFF or <NR1>=0 Disables the beeper
<b>Returns</b>	None
<b>Example</b>	SYSTem:BEEPer Generates an audible beep.

Table 166: SYSTem:BEEPer[:IMMEDIATE]

<b>Command</b>	SYSTem:DATE
----------------	-------------

<b>Description</b>	This command sets or returns the system date.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:DATE <yyyy>,<mm>,<dd> SYSTem:DATE?
<b>Related Commands</b>	None
<b>Arguments</b>	<year>::=<NR1> (Four digit number) <month>::=<NR1> from 1 to 12 <day>::=<NR1> from 1 to 31
<b>Returns</b>	<year>,<month>,<day>
<b>Example</b>	SYSTem:DATE 2018,11,20 Sets the date to November 20, 2018. SYSTem:DATE? Might return 2018,12,8.

**Table 167: SYSTem:DATE**

<b>Command</b>	SYSTem:ERROr[:NEXT]?
<b>Description</b>	This command returns data from the error and event queues.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:ERROr[:NEXT]?
<b>Related Commands</b>	None
<b>Arguments</b>	<Error number>, <error description> Error number ::=<NR1>. error description ::=<string>.
<b>Returns</b>	<year>,<month>,<day>
<b>Example</b>	SYSTem:ERROr:NEXT? Might return 0,"No error", indicating there are not errors.

**Table 168: SYSTem:ERROr[:NEXT]?**

<b>Command</b>	SYSTem:KLOCK[:STATE]
<b>Description</b>	This command locks or unlocks the instrument front panel controls. The query command returns "0" (OFF) or "1" (ON).
<b>Group</b>	System
<b>Syntax</b>	SYSTem:KLOCK[:STATE] {OFF   ON} SYSTem:KLOCK[:STATE]?
<b>Related Commands</b>	None
<b>Arguments</b>	ON or <NR1>#0 Locks front panel controls OFF or <NR1>=0

	Unlocks front panel controls
<b>Returns</b>	<NR1>
<b>Example</b>	SYSTem:KLOCK ON Locks front panel controls.

**Table 169: SYSTem:KLOCK[:STATe]**

<b>Command</b>	SYSTem:SECURITY:IMMEDIATE (No Query Form)
<b>Description</b>	This command erases all configurations and user waveforms and recalls the factory default settings. Calibration data is not erased.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:SECURITY:IMMEDIATE
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<NR1>
<b>Example</b>	SYSTem:SECURITY:IMMEDIATE Initializes the instrument.

**Table 170: SYSTem:SECURITY:IMMEDIATE**

<b>Command</b>	SYSTem:TIME
<b>Description</b>	This command sets or returns the system time (hours, minutes and seconds).
<b>Group</b>	System
<b>Syntax</b>	SYSTem:TIME <hh>,<mm>,<ss> SYSTem:TIME?
<b>Related Commands</b>	None
<b>Arguments</b>	<hour>,<minute>,<second> <hour> ::= <NR1> specifies the hours. Range: 0 to 23. <minute> ::= <NR1> specifies the minutes. Range: 0 to 59. <second> ::= <NR1> specifies the seconds. Range: 0 to 59.
<b>Returns</b>	<hour>,<minute>,<second> <hour> ::= <NR1> specifies the hours. <minute> ::= <NR1> specifies the minutes. <second> ::= <NR1> specifies the seconds.
<b>Example</b>	SYSTem:TIME 10,15,30 Sets the time to 10:15:30. SYSTem:TIME? Might return 12,20,32, indicating the system time is 12:20:32.

**Table 171: SYSTem:TIME**

<b>Command</b>	SYSTem:VERSion? (Query Only)
<b>Description</b>	This command returns the SCPI version number to which the command conforms.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:VERSion?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	A single <NR2> value. <NR2> ::= YYYY.V where YYYY is the year version and V is revision number for that year.
<b>Example</b>	SYSTem:VERSion? Might return 1999.0

**Table 172: SYSTem:VERSion**

## 6.14 TRIGGER GROUP COMMANDS

<b>Command</b>	ABORT (No Query Form)
<b>Description</b>	This command stops waveform playout when the Run Mode is set to Gated. This is equivalent to release the Force Trigger button on the front panel when the instrument is in gated mode
<b>Group</b>	Trigger
<b>Syntax</b>	ABORT
<b>Related Commands</b>	AWGControl:RMODE, *TRG
<b>Example</b>	ABORT It will stop the waveform playout on all channels with their Run Mode set to Gated.

**Table 173: ABORT**

<b>Command</b>	TRIGger[:SEQUence]:SOURce
<b>Description</b>	This command sets or returns the instrument trigger source.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence]:SOURce {TImer   EXternal   MANual} TRIGger[:SEQUence]:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	<source> ::= {TImer   EXternal   MANual} TImer: the trigger is sent at regular intervals of time. EXternal: the trigger come from the external BNC connector. MANual: the trigger is sent via software or using the trigger button on front panel.
<b>Returns</b>	TIM   EXT   MAN
<b>Example</b>	TRIGger:SOURce TImer It sets the trigger source to timer. TRIGger:SOURce? Might return TImer.

**Table 174: TRIGger[:SEQUence]:SOURCE**

<b>Command</b>	TRIGger[:SEQUence]:SLOPe
<b>Description</b>	This command sets or returns the instrument trigger input slope for the external source.
<b>Group</b>	Trigger

<b>Syntax</b>	TRIGger[:SEQUence]:SLOPe {POSitive   NEGative   BOTH} TRIGger[:SEQUence]:SLOPe?
<b>Related Commands</b>	TRIGger[:SEQUence]:SOURce
<b>Arguments</b>	<p>&lt;slope&gt; ::= {POSitive   NEGative   BOTH}</p> <p>POSitive specifies a trigger event on the rising edge of the external trigger signal.</p> <p>NEGative specifies a trigger event on the falling edge of the external trigger signal.</p> <p>BOTH specifies that a trigger event occurs both on falling and rising edge of the external trigger signal.</p>
<b>Returns</b>	<slope>
<b>Example</b>	<pre>TRIGger:SLOPe POS It sets the trigger slope to rising edge.  TRIGger:SLOPe? Might return BOTH.</pre>

Table 175: TRIGger[:SEQUence]:SLOPe

<b>Command</b>	TRIGger[:SEQUence]:LEVel
<b>Description</b>	This command sets or queries the threshold of the trigger-in signal.
<b>Group</b>	Trigger
<b>Syntax</b>	<pre>TRIGger[:SEQUence]:LEVel {MINimum   MAXimum   DEFault   &lt;Volts&gt;} TRIGger[:SEQUence]:LEVel? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	TRIGger[:SEQUence]:SOURce
<b>Arguments</b>	<p>&lt;Volts&gt; ::= &lt;NRf&gt; specifies the voltage threshold of external trigger-in signal.</p> <p>MINimum sets or queries the minimum threshold level.</p> <p>MAXimum sets or queries the maximum threshold level.</p> <p>DEFault sets the default threshold level (0V).</p>
<b>Returns</b>	<threshold>
<b>Example</b>	<pre>TRIGger:LEVel 5.5 Sets the external trigger-in threshold level to 5.5 V.  TRIGger:LEVel? MINimum It returns -10.</pre>

Table 176: TRIGger[:SEQUence]:LEVel

<b>Command</b>	TRIGger[:SEQUence]:TImer
----------------	--------------------------

<b>Description</b>	This command sets or queries the interval of an internal trigger-in event when you select TIMER as the trigger source with the TRIGger[:SEQUence]:SOURce command. The value will be automatically rounded to the closest time interval that the instrument is able to generate.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence]:TImer {MINimum   MAXimum   DEFault   <Seconds>} TRIGger[:SEQUence]:TImer? [{MINimum   MAXimum}]
<b>Related Commands</b>	TRIGger[:SEQUence]:SOURce
<b>Arguments</b>	<seconds>::=<NRf>[<units>] where: <units>::=[μs   ms   s] and it specifies the interval value expressed in <units>. MINimum sets or queries the minimum interval value. MAXimum sets or queries the maximum interval value. DEFault sets the default interval value (1 s).
<b>Returns</b>	<Seconds>
<b>Example</b>	TRIGger:TImer 300ms It sets the trigger-in interval to 0.3 seconds. The edited value is automatically rounded to the closest value that the hardware can implement. TRIGger:TImer? It might return 1.000000025 seconds.

**Table 177: TRIGger[:SEQUence]:TImer**

<b>Command</b>	TRIGger[:SEQUence]:TImer:RESETCondition
<b>Description</b>	This command sets or queries the condition which allows the timer to restart the time interval after which the trigger event is generated. The condition that reset the timer is specified in the command argument.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence]:TImer:RESETCondition {EXTERNAL   EXTMODInput}, {OFF   ON} TRIGger[:SEQUence]:TImer:RESETCondition? {EXTERNAL   EXTMODInput}
<b>Related Commands</b>	TRIGger[:SEQUence]:TImer
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• EXTERNAL: the timer is reset when an event on the external Trigger In signal occurs.</li> </ul>

	<ul style="list-style-type: none"> <li>• EXTMODInput: the timer is reset when an event on the external Ext Mod In signal occurs.</li> </ul> <p>Note: these conditions are not mutually exclusive, the command can be run multiple times with different arguments to create a combination between them.</p>
<b>Returns</b>	0 1 where '0' means that the specified condition is disabled and '1' means it's enabled
<b>Example</b>	<p>TRIGger:TIMER:RESETCondition EXTernal,ON      It means that the timer will be reset when an event on the external Trigger In occurs.</p> <p>TRIGger:TIMER:RESETCondition? EXTMODInput      It might return 1 which means that the condition to reset the timer when an event on Ext. Mod. In connector occurs is enabled.</p>

**Table 178: TRIGger[:SEQUence]:TIMER:RESETCondition**

<b>Command</b>	TRIGger:IMPedance
<b>Description</b>	This command sets or returns the trigger input impedance. It applies only to the external trigger signal (from BNC connector).
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger:IMPedance {50Ohm   1KOhm} TRIGger:IMPedance?
<b>Related Commands</b>	TRIGger[:SEQUence]:SOURce
<b>Arguments</b>	<impedance> ::= {50Ohm   1KOhm}
<b>Returns</b>	< impedance >
<b>Example</b>	<p>TRIGger:IMPedance 50Ohm      It sets the trigger impedance to 50 Ohm.</p> <p>TRIGger:IMPedance?      It might return 50 Ohm.</p>

**Table 179: TRIGger:IMPedance**

<b>Command</b>	TRIGger[:SEQUence][:IMMediate] (No Query Form)
<b>Description</b>	This command forces a trigger event to occur.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence][:IMMediate]
<b>Related Commands</b>	AWGControl:RMODE ABORT *TRG

<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	TRIGger:SEQUence:IMMEDIATE It generates a trigger event.

**Table 180: TRIGger[:SEQUence][:IMMEDIATE]**

<b>Command</b>	TRIGger[:SEQUence]:EXTMOD:ENABLE
<b>Description</b>	This command sets or returns the status of Ext. Mod. signal whose effects can be disabled while remaining connected to the Ext Mod In rear connector. <b>Note:</b> the events, generated by the Ext. Mod. Signal, are evaluated only if the Run Mode is set as Advanced.
<b>Group</b>	Control
<b>Syntax</b>	TRIGger[:SEQUence]:EXTMOD:ENABLE {<enable_value>} TRIGger[:SEQUence]:EXTMOD:ENABLE?
<b>Related Commands</b>	TRIGger[:SEQUence]:EXTMOD:Level TRIGger[:SEQUence]:EXTMOD:Slope
<b>Arguments</b>	<enable_value>:= {OFF   ON} <ul style="list-style-type: none"><li>• OFF: disables any event generated by Ext. Mod. signal.</li><li>• ON: enables the events generated by Ext. Mod. signal.</li></ul>
<b>Returns</b>	0   1 where '0' means OFF and '1' means ON
<b>Example</b>	TRIGger:EXTMOD:ENABLE ON Enables the events generated by Ext. Mod. signal. TRIGger:EXTMOD:ENABLE? Might return 1.

**Table 181: TRIGger[:SEQUence]:EXTMOD:ENABLE**

<b>Command</b>	TRIGger[:SEQUence]:EXTMOD:Level
<b>Description</b>	This command sets or queries the threshold of the Ext. Mod. signal.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence]:EXTMOD:Level {MINimum   MAXimum   DEFault   <Volts>} TRIGger[:SEQUence]:EXTMOD:Level? [{MINimum   MAXimum}]
<b>Related Commands</b>	TRIGger[:SEQUence]:EXTMOD:Slope
<b>Arguments</b>	<Volts>::= <NRf> specifies the voltage threshold of external Ext. Mod. signal.

	MINimum sets or queries the minimum threshold level. MAXimum sets or queries the maximum threshold level. DEFault sets the default threshold level (0V).
<b>Returns</b>	<EXTMOD threshold>
<b>Example</b>	TRIGger:EXTMOD:Level 0.5 Sets the threshold level of the external Ext. Mod. signal to 0.5 V. TRIGger:EXTMOD:Level? MINimum It returns -0.950V.

**Table 182: TRIGger[:SEQUence]:EXTMOD:Level**

<b>Command</b>	TRIGger[:SEQUence]:EXTMOD:Slope
<b>Description</b>	This command sets or returns the slope of Ext. Mod. input signal.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQUence]:EXTMOD:Slope {POSitive   NEGative} TRIGger[:SEQUence]:EXTMOD:Slope?
<b>Related Commands</b>	TRIGger[:SEQUence]:EXTMOD:Level
<b>Arguments</b>	<slope>::= {POSitive   NEGative} POSitive specifies a trigger event on the rising edge of the Ext. Mod. signal. NEGative specifies a trigger event on the falling edge of the Ext. Mod. signal.
<b>Returns</b>	<EXTMODslope>
<b>Example</b>	TRIGger:EXTMOD:Slope POS It sets the Ext. Mod. slope to rising edge. TRIGger:EXTMOD:Slope? Might return NEGative.

**Table 183: TRIGger[:SEQUence]:EXTMOD:Slope**

## 6.15 SEQUENCE GROUP COMMANDS

<b>Command</b>	SEQuence:ELEM[n]:AMPlitude[m]
<b>Description</b>	Sets or returns the voltage peak-to-peak amplitude for the element "n" of the channel "m"
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:AMPlitude[m] {MINimum   MAXimum   DEFault   <Volts>} SEQuence:ELEM[n]:AMPlitude[m]? [{MINimum   MAXimum}]
<b>Related Commands</b>	SEQuence:ELEM[n]:OFFset[m]
<b>Arguments</b>	The value of n indicates the sequence element number. The value of m is the channel number. <Volts>::=<NRf> sets the peak-to peak amplitude level expressed in Volt. MINimum sets or queries the minimum amplitude level. MAXimum sets or queries the maximum amplitude level. DEFault sets the default amplitude level (2V).
<b>Returns</b>	<Volts>::=<NRf>
<b>Example</b>	SEQuence:ELEM3:AMPlitude2 4 Sets the voltage amplitude of the channel 2 for sequencer element 3 to 4V. SEQuence:ELEM3:AMPlitude2? Might return 4.

**Table 184: SEQuence:ELEM[n]:AMPlitude[m]**

<b>Command</b>	SEQuence:ELEM[n]:OFFset[m]
<b>Description</b>	Sets or returns the voltage offset for the element "n" of the channel "m"
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:OFFset[m] {MINimum   MAXimum   DEFault   <Volts>} SEQuence:ELEM[n]:OFFset[m]? [{MINimum   MAXimum}]
<b>Related Commands</b>	SEQuence:ELEM[n]:AMPlitude[m]
<b>Arguments</b>	The value of n indicates the sequence element number. The value of m is the channel number. <Volts>::=<NRf> sets the offset level expressed in Volt. MINimum sets or queries the minimum offset level. MAXimum sets or queries the maximum offset level.

	DEFault sets the default offset level (0V).
<b>Returns</b>	<Volts>::=<NRF>
<b>Example</b>	<p>SEQuence:ELEM5:OFFset2 1.2          Sets the offset of the channel 2 for sequencer element 5 to 1.2 V.          SEQuence:ELEM5:OFFset2? MAXimum          Might return 2.5.</p>

**Table 185: SEQuence:ELEM[n]:OFFset[m]**

<b>Command</b>	SEQuence:ELEM[n]:VOLTage:HIGH[m]
<b>Description</b>	This command sets or returns the high voltage level of the waveform for the element “n” of the channel “m”.
<b>Group</b>	Sequence
<b>Syntax</b>	<p>SEQuence:ELEM[n]:VOLTage:HIGH[m] {MINimum   MAXimum   DEFault   &lt;Volts&gt;}</p> <p>SEQuence:ELEM[n]:VOLTage:HIGH[m]? [{MINimum   MAXimum}]</p>
<b>Related Commands</b>	SEQuence:ELEM[n]:VOLTage:LOW[m]
<b>Arguments</b>	<p>The value of n indicates the sequence element number.          The value of m is the channel number.          &lt;Volts&gt;::=&lt;NRF&gt; sets the is the high level of output amplitude expressed in Volt.          MINimum sets or queries the minimum value of high voltage level.          MAXimum sets or queries the maximum value of high voltage level.          DEFault sets the default value of high voltage level (1V).</p>
<b>Returns</b>	<Volts>::=<NRF>
<b>Example</b>	<p>SEQuence:ELEM2:VOLTage:HIGH1 2.3          Sets the high level voltage of the channel 1 for sequencer element 2 to 2.3 V.          SEQuence:ELEM2:VOLTage:HIGH1?          Might return 2.3.</p>

**Table 186: SEQuence:ELEM[n]:VOLTage:HIGH[m]**

<b>Command</b>	SEQuence:ELEM[n]:VOLTage:LOW[m]
<b>Description</b>	This command sets or returns the low voltage level of the waveform for the element “n” of the channel “m”.
<b>Group</b>	Sequence
<b>Syntax</b>	<p>SEQuence:ELEM[n]:VOLTage:LOW[m] {MINimum   MAXimum   DEFault   &lt;Volts&gt;}</p> <p>SEQuence:ELEM[n]:VOLTage:LOW[m]? [{MINimum   MAXimum}]</p>

<b>Related Commands</b>	SEQuence:ELEM[n]:VOLTage:HIGH[m]
<b>Arguments</b>	<p>The value of n indicates the sequence element number.</p> <p>The value of m is the channel number.</p> <p>&lt;Volts&gt;::=&lt;NRf&gt; sets the low level of output amplitude expressed in Volt.</p> <p>MINimum sets or queries the minimum value of low voltage level.</p> <p>MAXimum sets or queries the maximum value of low voltage level.</p> <p>DEFault sets the default value of low voltage level (-1V).</p>
<b>Returns</b>	<Volts>::=<NRf>
<b>Example</b>	<p>SEQuence:ELEM2:VOLTage:LOW2 -1.7</p> <p>Sets the low level voltage of the channel 2 for sequencer element 2 to -1.7 V.</p> <p>SEQuence:ELEM1:VOLTage:LOW3? MINimum</p> <p>Might return -6.</p>

**Table 187: SEQuence:ELEM[n]:VOLTage:LOW[m]**

<b>Command</b>	SEQuence:ELEM[n]:LENGth
<b>Description</b>	This command sets or returns the number of samples of the waveform for the element “n”.
<b>Group</b>	Sequence
<b>Syntax</b>	<p>SEQuence:ELEM[n]:LENGth {MINimum   MAXimum   DEFault   &lt;value&gt;}</p> <p>SEQuence:ELEM[n]:LENGth? [{MINimum   MAXimum}]</p>
<b>Related Commands</b>	None
<b>Arguments</b>	<p>The value of n indicates the sequence element number.</p> <p>&lt;value&gt;::=&lt;NR1&gt; is the length of entry n.</p> <p>MINimum sets or queries the minimum value of length.</p> <p>MAXimum sets or queries the maximum value of length.</p> <p>DEFault sets the default value of length (16384).</p>
<b>Returns</b>	<value>::=<NR1>
<b>Example</b>	<p>SEQuence:ELEM3:LENGth 1000</p> <p>Sets the number of waveform's samples of the element 3 to 1000 for all channels.</p> <p><b>NOTE:</b> The set value is automatically rounded to the closest value that the hardware can implement compatibly with granularity.</p> <p>SEQuence:ELEM2:LENGth?</p> <p>Might return 1000.</p>

**Table 188: SEQuence:ELEM:LENgth**

<b>Command</b>	SEQuence:ELEM[n]:LOOP:COUNT
<b>Description</b>	This command sets or returns the number of repetitions of the waveform for the element “n”.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:LOOP:COUNT {MINimum   MAXimum   DEFault   INFinite   <value>} SEQuence:ELEM[n]:LOOP:COUNT? [{MINimum   MAXimum}]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the sequence element number. <value>::=<NR1> is the number of repetitions of entry n. MINimum sets or queries the minimum value of repetitions parameter. MAXimum sets or queries the maximum value of repetitions parameter. INFinite sets infinite repetitions. DEFault sets the default value of repetition (1).
<b>Returns</b>	<value>::=<NR1>
<b>Example</b>	SEQUENCE:ELEM1:LOOP:COUNT 120 Sets the repetitions parameter of the element 1 to 120 for all channels SEQUENCE:ELEM1:LOOP:COUNT? MAXimum It returns 4294967295.

**Table 189: SEQuence:ELEM[n]:LOOP:COUNT**

<b>Command</b>	SEQuence:ELEM[n]:WAVEform[m]
<b>Description</b>	This command sets or returns the waveform for the sequence element “n”. The value of “m” indicates the channel that will output the waveform when the sequence is run. It's possible select a waveform only from those in the waveform list. In waveform list are already present 14 predefined waveform: Sine, Ramp, Square, Sync, DC, Gaussian, Lorentz, Haversine, Exp_Rise, Exp_Decay, Zero, One, Clock and Counter but user can import in the list others customized waveforms or create parametric waveforms.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:WAVEform[m] <wfm_name> SEQuence:ELEM[n]:WAVEform[m]?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the element index.

	The value of m is the channel number. <wfm_name>::=<String> is the waveform's name.
<b>Returns</b>	<wfm_name>::=<String>
<b>Example</b>	SEQUENCE:ELEM1:WAVEFORM1 "TRIANGLE1000" Sets the "TRIANGLE1000" waveform into the first element of the sequence of channel 1. SEQuence:ELEM3:WAveform1? Might return SQUARE.

**Table 190: SEQuence:ELEM[n]:WAveform[m]**

<b>Command</b>	SEQuence:LENGTH
<b>Description</b>	This command sets or returns the entire sequence length. Also note that passing a value less than the sequence's current length will cause some elements to be deleted at the end of the sequence. For example if SEQuence:LENGTH? returns 100 and you subsequently send SEQuence:LENGTH 20, all sequence elements except the first 20 will be deleted.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:LENGTH {MINimum   MAXimum   DEFault   <value>} SEQuence:LENGTH?
<b>Related Commands</b>	None
<b>Arguments</b>	<value>::=<NR1> it is the sequence length. The MINimum and DEFault parameters will set a length = 1, MAXimum parameter will set a length = 16384.
<b>Returns</b>	<value>::=<NR1>
<b>Example</b>	SEQuence:LENGTH 50 Sets the sequencer length to 50 entries for all channels initializing all sequence parameters to default values. SEQuence:LENGTH? Might return 50.

**Table 191: SEQuence:LENGTH**

<b>Command</b>	SEQuence:NEW (No Query Form)
<b>Description</b>	This command creates a new sequence with only one element with default value.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:NEW
<b>Related Commands</b>	None

<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	SEQuence:NEW It creates a new sequence (with only one element).

Table 192: SEQuence:NEW

<b>Command</b>	SEQuence:FOCUS (No Query Form)
<b>Description</b>	This command visualizes a specific element of the sequencer on the display.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:FOCUS {MINimum   MAXimum   DEFault   <value>}
<b>Related Commands</b>	None
<b>Arguments</b>	<value> ::= <NR1> indicates the element to visualize. MINimum and DEFault set the first element of the sequencer to be displayed. MAXimum sets the last element of the sequencer to be displayed.
<b>Returns</b>	None
<b>Example</b>	SEQuence:FOCUS 5 The fifth element of the sequencer will be displayed.

Table 193: SEQuence:FOCUS

<b>Command</b>	SEQuence:ELEM[n]:WAITEvent
<b>Description</b>	This command sets or returns the wait event type for the selected element 'n'.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:WAITEvent {NONE   MANUAL   TIMER   EXTERNAL   EXTMODINPUT} SEQuence:ELEM[n]:WAITEvent?
<b>Related Commands</b>	None
<b>Arguments</b>	<wait_event> ::= {NONE   MANUAL   TIMER   EXTERNAL   EXTMODINPUT} NONE: the wait event is disabled. MANUAL: the wait event is sent via software or by pressing the front panel button. TIMER: the wait event is generated by an internal timer. EXTERNAL: the wait event comes from the external BNC connector EXTMODINPUT: the wait event comes from the external rear SMA connector Ext Mod In.

<b>Returns</b>	<wait_event> ::= {NONE   MANUAL   TIMER   EXTERNAL   EXTMODINPUT}
<b>Example</b>	<p>SEQuence:ELEM1:WAITEvent TIMER      It sets the wait event for first element of the sequence to timer.      SEQuence:ELEM1:WAITEvent?      Might return TIMER.</p>

**Table 194: SEQuence:ELEM[n]:WAITEvent**

<b>Command</b>	SEQuence:ELEM[n]:GOTOMode
<b>Description</b>	<p>This command sets or returns the “GOTO” command type for the selected element ‘n’ of the sequencer.</p> <p>After generating the waveform(s) specified in a sequence element, the sequencer jumps to the entry specified as the GOTO Item. This is an unconditional jump.</p>
<b>Group</b>	Sequence
<b>Syntax</b>	<p>SEQuence:ELEM[n]:GOTOMode {FIRST   PREVIOUS   NEXT   LAST   ITEM}      SEQuence:ELEM[n]:GOTOMode?</p>
<b>Related Commands</b>	SEQuence:ELEM[n]:GOTOEntry
<b>Arguments</b>	<p>&lt;mode&gt; ::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }</p> <p>FIRST: the sequencer will go to the first element of the sequence</p> <p>PREVIOUS: the sequencer will go to the previous element of the sequence. If the selected element is the first, it will jump to the last.</p> <p>NEXT: the sequencer will go to the next element of the sequence. If the selected element is the last, it will jump to the first.</p> <p>ITEM: the sequencer will go to the selected item of the sequencer defined in the command SEQuence:ELEM[n]:GOTOEntry</p>
<b>Returns</b>	<mode> ::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }
<b>Example</b>	<p>SEQuence:ELEM4:GOTOMode FIRST      The sequencer will jump to the first element after executing the fourth element.      SEQuence:ELEM4:GOTOMode?      Might return FIRST.</p>

**Table 195: SEQuence:ELEM[n]:GOTOMode**

<b>Command</b>	SEQuence:ELEM[n]:GOTOEntry
<b>Description</b>	This command sets or returns the target entry for the “GOTO” command for the selected element ‘n’ of the sequencer.

	After generating the waveform(s) specified in a sequence element, the sequencer jumps to the entry specified as the GOTO target. This is an unconditional jump.
<b>Group</b>	Sequence
<b>Syntax</b>	<pre>SEQuence:ELEM[n]:GOTOEntry {MINimum   MAXimum   DEFault   &lt;value&gt;}</pre> <pre>SEQuence:ELEM[n]:GOTOEntry? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	SEQuence:ELEM[n]:GOTOMode
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; value &gt; ::= &lt;NR1&gt; sets the target entry index</li> </ul>
<b>Returns</b>	< value > ::= <NR1>
<b>Example</b>	<pre>SEQuence:ELEM4:GOTOMode ITEM SEQuence:ELEM4:GOTOEntry 2</pre> <p>The sequencer will jump to the second entry of the sequencer after executing the fourth element.</p> <pre>SEQuence:ELEM4:GOTOEntry? Might return 2.</pre>

**Table 196: SEQuence:ELEM[n]:GOTOEntry**

<b>Command</b>	SEQuence:ELEM[n]:JUMPTOMode
<b>Description</b>	This command sets or returns the “Jump To” command type for the selected element ‘n’ of the sequencer.  The “Jump To” command is a conditional jump.
<b>Group</b>	Sequence
<b>Syntax</b>	<pre>SEQuence:ELEM[n]:JUMPTOMode {FIRST   PREVIOUS   NEXT   LAST   ITEM}</pre> <pre>SEQuence:ELEM[n]:JUMPTOMode?</pre>
<b>Related Commands</b>	SEQuence:ELEM[n]:JUMPTOEntry SEQuence:ELEM[n]:JUMPEvent

	AWGControl:JUMPMODE
<b>Arguments</b>	<p>&lt;mode&gt; ::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }</p> <p>FIRST: the sequencer will jump to the first element of the sequence</p> <p>PREVIOUS: the sequencer will jump to the previous element of the sequence. If the selected element is the first, it will jump to the last.</p> <p>NEXT: the sequencer will jump to the next element of the sequence. If the selected element is the last, it will jump to the first.</p> <p>ITEM: the sequencer will jump to the selected item of the sequencer defined in the command SEQuence:ELEM[n]:JUMPTOEntry</p>
<b>Returns</b>	<mode> ::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }
<b>Example</b>	<p>SEQuence:ELEM4:JUMPTOMode LAST</p> <p>The sequencer will jump to the last element after the jump event occurs.</p> <p>SEQuence:ELEM4:JUMPTOMode?</p> <p>Might return LAST.</p>

**Table 197: SEQuence:ELEM[n]:JUMPTOMode**

<b>Command</b>	SEQuence:ELEM[n]:JUMPEvent
<b>Description</b>	This command sets or returns the jump event type for the selected element 'n'.
<b>Group</b>	Sequence
<b>Syntax</b>	<p>SEQuence:ELEM[n]:JUMPEvent {NONE   MANual   TImer   EXternal   EXTModInPut}</p> <p>SEQuence:ELEM[n]:JUMPEvent?</p>
<b>Related Commands</b>	<p>SEQuence:ELEM[n]:JUMPTOEntry</p> <p>SEQuence:ELEM[n]:JUMPTOMode</p> <p>AWGControl:JUMPMODE</p>
<b>Arguments</b>	<p>&lt;jump_event&gt; ::= {NONE   MANual   TImer   EXternal   EXTModInPut}</p> <p>NONE: the jump event is disabled.</p> <p>MANual: the jump event is sent via software or by pressing the front panel button.</p> <p>TImer: the jump event is generated by an internal timer.</p> <p>EXternal: the jump event comes from the external BNC connector</p> <p>EXTModInPut: the jump event comes from the external rear SMA connector Ext Mod In.</p>
<b>Returns</b>	<jump_event> ::= {NONE   MANual   TImer   EXternal   EXTModInPut}
<b>Example</b>	<p>SEQuence:ELEM1: JUMPEvent MANual</p> <p>It sets the jump event for first element of the sequence to manual.</p>

	SEQuence:ELEM1:JUMPEvent? Might return MANual.
--	---

**Table 198: SEQuence:ELEM[n]:JUMPEvent**

<b>Command</b>	SEQuence:ELEM[n]:JUMPTOEntry
<b>Description</b>	<p>This command sets or returns the target entry index for the “Jump To” command for the selected element ‘n’ of the sequencer.</p> <p>After generating the waveform(s) specified in a sequence element, the sequencer jumps to the entry specified as the “Jump To” target index after the event occurs. This is a conditional jump.</p> <p>Note: this will take effect only when SEQuence:ELEM[n]:JUMPTOMode is set to ITEM.</p>
<b>Group</b>	Sequence
<b>Syntax</b>	<pre>SEQuence:ELEM[n]:JUMPTOEntry {MINimum   MAXimum   DEFault   &lt;value&gt;}</pre> <pre>SEQuence:ELEM[n]:JUMPTOEntry? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	SEQuence:ELEM[n]:JUMPEvent SEQuence:ELEM[n]:JUMPTOMode AWGControl:JUMPMODE
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; value &gt;:= &lt;NR1&gt; sets the target entry index</li> </ul>
<b>Returns</b>	< value > := <NR1>
<b>Example</b>	<pre>SEQuence:ELEM4:JUMPTOMode ITEM SEQuence:ELEM4:JUMPTOEntry 6 Sets the jump target entry index to the 6<sup>th</sup> element.</pre> <pre>SEQuence:ELEM4:JUMPTOEntry? Might return 6.</pre>

**Table 199: SEQuence:ELEM[n]:JUMPTOEntry**

<b>Command</b>	SEQuence:ELEM[n]:PATTERNEvent
----------------	-------------------------------

<b>Description</b>	<p>This command sets or returns the Pattern Jump event type for the selected element 'n'.</p> <p>It belongs to the family of "pattern jump" commands. The "pattern jump" is a dynamic jump that occurs when a Pattern code is received by the sequencer or due to an event on the Ext Mod in SMA connector.</p> <p><b>Note:</b> if, for the same entry, the JUMPEvent and PATTERNEvent parameters are both set with the EXTMODInput option, the generation flow will jump to the entry set by PATTERNJUMPTOMode parameter. This happens because the dynamic jumps (and the related settings) have a greater relevance than the conditional ones.</p>
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:PATTERNEvent {PATTERN   EXTMODInput} SEQuence:ELEM[n]:PATTERNEvent?
<b>Related Commands</b>	SEQuence:ELEM[n]:PATTERN SEQuence:ELEM[n]:PATTERNJUMPTOMode SEQuence:ELEM[n]:PATTERNJUMPTOEntry AWGControl:DJStrobe
<b>Arguments</b>	<p>&lt;pattern_jump_event&gt; ::= {PATTERN   EXTMODInput}</p> <p>PATTERN: the pattern jump event is generated via a SCPI command (AWGControl:DJStrobe) after setting a pattern code.</p> <p>EXTMODInput: the pattern jump event comes from the external rear SMA connector Ext Mod In.</p>
<b>Returns</b>	<pattern_jump_event> ::= {PATTERN   EXTMODInput}
<b>Example</b>	<p>SEQuence:ELEM2:PATTERNEvent PATTERN</p> <p>It sets the Pattern Jump event for second element of the sequence to pattern.</p> <p>SEQuence:ELEM1:PATTERNEvent?</p> <p>Might return EXTMODInput.</p>

Table 200: SEQuence:ELEM[n]:PATTERNEvent

<b>Command</b>	SEQuence:ELEM[n]:PATTERN
<b>Description</b>	This command sets or returns the pattern code value for the "Pattern Jump" command for the selected element 'n' of the sequencer.

	<p>It belongs to the family of “pattern jump” commands. The “pattern jump” is a dynamic jump.</p> <p><b>Note:</b> this command sets the pattern code value, while the pattern is sent by using the command AWGControl:DJStrobe</p>
<b>Group</b>	Sequence
<b>Syntax</b>	<pre>SEQuence:ELEM[n]:PATTERN {MINimum   MAXimum   DEFault   &lt;value&gt;} SEQuence:ELEM[n]:PATTERN? [{MINimum   MAXimum}]</pre>
<b>Related Commands</b>	<pre>SEQuence:ELEM[n]:PATTERNJUMPTOMode SEQuence:ELEM[n]:PATTERNJUMPTOEntry AWGControl:DJStrobe</pre>
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; value &gt; := &lt;NR1&gt; sets the pattern code value</li> </ul>
<b>Returns</b>	<value>::=<NR1>
<b>Example</b>	<pre>SEQuence:ELEM1:PATTERN 123 It sets the pattern code to 123 for first element of the sequence . SEQuence:ELEM1:PATTERN? Might return 123.</pre>

Table 201: SEQuence:ELEM[n]:PATTERN

<b>Command</b>	SEQuence:ELEM[n]:PATTERNJUMPTOMode
<b>Description</b>	<p>This command sets or returns the “Pattern Jump” command type for the selected element ‘n’ of the sequencer.</p> <p>It belongs to the family of “pattern jump” commands. The “pattern jump” command is a dynamic jump.</p>
<b>Group</b>	Sequence
<b>Syntax</b>	<pre>SEQuence:ELEM[n]:PATTERNJUMPTOMode {FIRST   PREVIOUS   NEXT   LAST   ITEM} SEQuence:ELEM[n]:PATTERNJUMPTOMode?</pre>
<b>Related Commands</b>	<pre>SEQuence:ELEM[n]:PATTERN SEQuence:ELEM[n]:PATTERNJUMPTOEntry AWGControl:DJStrobe</pre>
<b>Arguments</b>	<pre>&lt;mode&gt;::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }</pre> <p>FIRST: the sequencer will jump to the first element of the sequence</p>

	PREVIOUS: the sequencer will jump to the previous element of the sequence. If the selected element is the first, it will jump to the last. NEXT: the sequencer will jump to the next element of the sequence. If the selected element is the last, it will jump to the first. ITEM: the sequencer will jump to the selected item of the sequencer defined in the command SEQuence:ELEM[n]: PATTERNJUMPTOEntry.
<b>Returns</b>	<mode> ::= { FIRST   PREVIOUS   NEXT   LAST   ITEM }
<b>Example</b>	SEQuence:ELEM4:PATTERNJUMPTOMode LAST The sequencer will jump to the last element after the pattern jump event occurs. SEQuence:ELEM4:PATTERNJUMPTOMode? Might return LAST.

**Table 202: SEQuence:ELEM[n]:PATTERNJUMPTOMode**

<b>Command</b>	SEQuence:ELEM[n]:PATTERNJUMPTOEntry
<b>Description</b>	This command sets or returns the target entry index for the “Pattern Jump To” command for the selected element ‘n’ of the sequencer.  It belongs to the family of “pattern jump” commands. The “pattern jump” is a dynamic jump.  <b>Note:</b> this will take effect only when SEQuence:ELEM[n]: PATTERNJUMPTOMode is set to ITEM.
<b>Group</b>	Sequence
<b>Syntax</b>	SEQuence:ELEM[n]:JUMPTOEntry {MINimum   MAXimum   DEFault   <value>} SEQuence:ELEM[n]:JUMPTOEntry? [{MINimum   MAXimum}]
<b>Related Commands</b>	SEQuence:ELEM[n]:PATTERN SEQuence:ELEM[n]:PATTERNJUMPTOEntry AWGControl:DJStrobe
<b>Arguments</b>	<ul style="list-style-type: none"> <li>• MINimum: sets the parameter to the minimum value</li> <li>• MAXimum: sets the parameter to the maximum value</li> <li>• DEFault: sets the parameter to the default value</li> <li>• &lt; value &gt; := &lt;NR1&gt; sets the target entry index</li> </ul>
<b>Returns</b>	< value > := <NR1>
<b>Example</b>	SEQuence:ELEM4:PATTERNJUMPTOMode ITEM Sets the pattern jump command type to Item SEQuence:ELEM4:PATTERNJUMPTOEntry 8

Sets the pattern jump target entry index to the 8<sup>th</sup> element.

SEQuence:ELEM4:JUMPTOEntry?

Might return 8.

Table 203: SEQuence:ELEM[n]:PATTERNJUMPTOEntry

## 6.16 WAVEFORM GROUP COMMANDS

<b>Command</b>	WLIST:LIST? (Query Only)
<b>Description</b>	This command returns the name of the all waveforms in the waveform list.
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:LIST?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	[<waveform_name>][,<waveform_name>]... <waveform_name>::=<string>
<b>Example</b>	WLIST:LIST? Might return "Sine, Ramp, Square, Sync, DC, Gaussian, Lorentz, Haversine, Exp_Rise, Exp_Decay, Zero, One, Counter, Clock, Waveform_Imported1, Waveform_imported2"

**Table 204: WLIST:LIST**

<b>Command</b>	WLIST:NAME? (Query Only)
<b>Description</b>	This command returns the waveform name from the waveform list at the position specified by the index value.
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:NAME? <Index>
<b>Related Commands</b>	None
<b>Arguments</b>	<Index>::=<NR1>
<b>Returns</b>	<string>::=<wfm_name> is the waveform name specified by <index>.
<b>Example</b>	WLIST:NAME? 21 Might return "waveform21".

**Table 205: WLIST:NAME**

<b>Command</b>	WLIST:SIZE? (Query Only)
<b>Description</b>	This query returns the size (number of waveforms) of the waveform list. Names of both predefined and user-imported waveforms are stored in a single list.
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:SIZE?
<b>Related Commands</b>	None
<b>Arguments</b>	None

<b>Returns</b>	<NR1> At *RST, this returns the number of predefined waveforms.
<b>Example</b>	WLIST:SIZE? Might return 14.

**Table 206: WLIST:SIZE?**

<b>Command</b>	WLIST:WAVeform:DATA? (Query Only)																																																																																
<b>Description</b>	<p>This command returns all sample of an analog or digital waveform (or a portion of them specifying StartIndex and Size parameters). In this way it possible transfer a waveform from the waveform list to the external control program.</p> <p>The returned bytes represent the waveform's sample. For analog waveforms every samples consists of 2 bytes while for digital ones of 4 bytes.</p> <p>In particular for analog waveform:</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td colspan="8">Analog waveform sample – 16 bits format (DAC's sample)</td> </tr> <tr> <td>byte offset 1</td><td>byte offset 0</td><td> </td><td> </td><td> </td><td> </td><td> </td><td> </td></tr> </table> <p>In particular for digital waveform:</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td colspan="8">Digital Waveform Sample</td> </tr> <tr> <td>byte offset 3</td><td>byte offset 2</td><td>byte offset 1</td><td>byte offset 0</td><td> </td><td> </td><td> </td><td> </td></tr> <tr> <td><b>Digital Pod D</b></td><td><b>Digital Pod C</b></td><td><b>Digital Pod B</b></td><td><b>Digital Pod A</b></td><td> </td><td> </td><td> </td><td> </td></tr> </table> <p>Digital Pod A</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>A(7)</td><td>A(6)</td><td>A(5)</td><td>A(4)</td><td>A(3)</td><td>A(2)</td><td>A(1)</td><td>A(0)/M(0)</td> </tr> </table> <p>Digital Pod B</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>B(7)</td><td>B(6)</td><td>B(5)</td><td>B(4)</td><td>B(3)</td><td>B(2)</td><td>B(1)</td><td>B(0)/M(1)</td> </tr> </table> <p>Digital Pod C</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>C(7)</td><td>C(6)</td><td>C(5)</td><td>C(4)</td><td>C(3)</td><td>C(2)</td><td>C(1)</td><td>C(0)/M(2)</td> </tr> </table> <p>Digital Pod D</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>D(7)</td><td>D(6)</td><td>D(5)</td><td>D(4)</td><td>D(3)</td><td>D(2)</td><td>D(1)</td><td>D(0)/M(3)</td> </tr> </table> <p>The order of bytes uses the little-endian format.</p>									Analog waveform sample – 16 bits format (DAC's sample)								byte offset 1	byte offset 0							Digital Waveform Sample								byte offset 3	byte offset 2	byte offset 1	byte offset 0					<b>Digital Pod D</b>	<b>Digital Pod C</b>	<b>Digital Pod B</b>	<b>Digital Pod A</b>					A(7)	A(6)	A(5)	A(4)	A(3)	A(2)	A(1)	A(0)/M(0)	B(7)	B(6)	B(5)	B(4)	B(3)	B(2)	B(1)	B(0)/M(1)	C(7)	C(6)	C(5)	C(4)	C(3)	C(2)	C(1)	C(0)/M(2)	D(7)	D(6)	D(5)	D(4)	D(3)	D(2)	D(1)	D(0)/M(3)
Analog waveform sample – 16 bits format (DAC's sample)																																																																																	
byte offset 1	byte offset 0																																																																																
Digital Waveform Sample																																																																																	
byte offset 3	byte offset 2	byte offset 1	byte offset 0																																																																														
<b>Digital Pod D</b>	<b>Digital Pod C</b>	<b>Digital Pod B</b>	<b>Digital Pod A</b>																																																																														
A(7)	A(6)	A(5)	A(4)	A(3)	A(2)	A(1)	A(0)/M(0)																																																																										
B(7)	B(6)	B(5)	B(4)	B(3)	B(2)	B(1)	B(0)/M(1)																																																																										
C(7)	C(6)	C(5)	C(4)	C(3)	C(2)	C(1)	C(0)/M(2)																																																																										
D(7)	D(6)	D(5)	D(4)	D(3)	D(2)	D(1)	D(0)/M(3)																																																																										

	<p>It is suggested that the user make use of the StartIndex and Size to append data in multiple queries.</p> <p>Using StartIndex and Size, part of a waveform can be transferred at a time. Very large waveforms can be transferred in chunks.</p> <p>Transferring large waveforms in chunks allows external programs to cancel the operation before it is completed.</p>
<b>Group</b>	Waveform
<b>Syntax</b>	WLSt:WAVEform:DATA? <wfm_name>[,<StartIndex>[,<Size>]]
<b>Related Commands</b>	None
<b>Arguments</b>	<p>&lt;wfm_name&gt; ::= &lt;string&gt; is the waveform's name in waveform list.</p> <p>&lt;StartIndex&gt; ::= &lt;NR1&gt; specifies the start byte</p> <p>&lt;Size&gt; ::= &lt;NR1&gt; specifies the number of bytes to return.</p>
<b>Returns</b>	<block_data> ::= IEEE 488.2 block data format
<b>Example</b>	<pre>WLSt:WAVEform:DATA? "TestWfm",0,1024</pre> <p>Returns #41024XXXX... where XXXX... are the first 1024 bytes of the waveform called "TestWfm".</p>

Table 207: WLSt:WAVEform:DATA

<b>Command</b>	WLSt:WAVEform:DElete (No Query Form)
<b>Description</b>	<p>This command deletes a specified waveform (or all waveforms) from the currently waveform list.</p> <p>If ALL is specified, all waveforms will be deleted except DC, SINE and ZERO waveforms.</p> <p>The operation is executed on current configuration only.</p> <p>If the deleted waveform is currently loaded into waveform memory, it is unloaded.</p> <p><b>Important Note:</b> When ALL is specified, all deletable waveforms in the database will be deleted in a single action. Note that there is no "UNDO" action once the waveforms are deleted. Use caution before issuing this command.</p> <p><b>NOTE:</b> The AWG must be in idle state.</p>
<b>Group</b>	Waveform
<b>Syntax</b>	WLSt:WAVEform:DElete {<wfm_name>   ALL}
<b>Related Commands</b>	<p>WLSt:SIZE?</p> <p>WLSt:NAME?</p>

<b>Arguments</b>	<wfm_name>::=<string>
<b>Returns</b>	None
<b>Example</b>	<pre>WLIST:WAveform:DElete ALL Deletes all waveforms from the waveform list except 'DC', 'SINE' and 'ZERO'. WLIST:WAveform:DELETE "Test1" Deletes a waveform called "Test1".</pre>

**Table 208: WLIST:WAveform:DElete**

<b>Command</b>	WLIST:WAveform:IMPort
<b>Description</b>	<p>This command imports the waveform from internal driver or USB driver into the waveform list.</p> <p>File formats supported:</p> <ul style="list-style-type: none"> <li>TXT: a list of numbers</li> <li>BIN: binary file</li> <li>TRC: Lecroy format</li> <li>ZIP: file archive property format.</li> </ul> <p><b>NOTE 1:</b> If waveform file has ".zip" extension then the parameter {ANALog   DIGitals} will not be taken into account. The ".zip" format already has this information in itself.</p> <p><b>NOTE 2:</b> If the waveform name is already present in the waveform list then an error will occur.</p> <p><b>NOTE 3:</b> If the waveform type {ANALog   DIGitals} is not specified, the ANALog type will be assumed as default.</p> <p><b>NOTE 4:</b> Only removable units and "C:\Users\&lt;username&gt;\Pictures\Saved Pictures" directory are accessible by this command. The waveform path may contain a full file path. However, if the file path only contains a waveform name, the waveform will be searched starting from the current directory.</p> <p><b>NOTE 5:</b> This operation is equivalent to what the user can do through the following user interface menu: Wave. List -&gt; Import</p>
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:WAveform:IMPort <wfm_name>,<file_name>[,{ANALog

	DIGItals}]
<b>Related Commands</b>	WLSt:SIZE? WLSt:NAME? WLSt:WAveform:DElete
<b>Arguments</b>	<wfm_name>::=<string> <file_name>::=<string>. {zip   trc   txt   bin} indicates the absolute or relative path of the waveform file to import. ANALog: the waveform is imported as analog waveform DIGItals: the waveform is imported as digitals waveform
<b>Returns</b>	None
<b>Example</b>	WLSt:WAveform:IMPort "MyImportedWave", "E:/WaveLib/Test1.txt", ANALog  Imports a waveform called "Test1.txt" located in E:/WaveLib directory in waveform list; it will be called "MyImportedWave" and it will appear as analog waveform.

**Table 209: WLSt:WAveform:IMPort**

<b>Command</b>	WLSt:WAveform:LMAXimum? (Query Only)
<b>Description</b>	This command returns the maximum number of waveform sample points allowed. The returned value is dependent on the instrument model and the installed options.
<b>Group</b>	Waveform
<b>Syntax</b>	WLSt:WAveform:LMAXimum?
<b>Related Commands</b>	WLSt:WAveform:LMINimum?
<b>Arguments</b>	None
<b>Returns</b>	<NR1>
<b>Example</b>	WLSt:WAveform:LMAXimum? Returns 1073741428 (if 1G option is installed)

**Table 210: WLSt:WAveform:LMAXimum?**

<b>Command</b>	WLSt:WAveform:LMINimum? (Query Only)
<b>Description</b>	This command returns the minimum number of waveform sample points required for a valid waveform.
<b>Group</b>	Waveform

<b>Syntax</b>	WLIST:WAveform:LMinimum?
<b>Related Commands</b>	WLIST:WAveform:LMaximum?
<b>Arguments</b>	None
<b>Returns</b>	<NR1>
<b>Example</b>	WLIST:WAveform:LMinimum? Returns 16.

**Table 211: WLIST:WAveform:LMinimum?**

<b>Command</b>	WLIST:WAveform:LENGth? (Query Only)
<b>Description</b>	This query returns the size of the waveform. The returned value represents data points (not bytes).
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:WAveform:LENGth? <wfm_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<wfm_name>::=<string>
<b>Returns</b>	<NR1>
<b>Example</b>	WLIST:WAveform:LENGth? "Sine_360samples" Might return 360 indicating that the waveform contains 360 samples.

**Table 212: WLIST:WAveform:LENGth?**

<b>Command</b>	WLIST:WAveform:PREDefined? (Query Only)
<b>Description</b>	This query returns true or false based on whether the waveform is predefined.  <b>Important Note:</b> Predefined waveforms have fixed length and name. Therefore, renaming or deleting them is not possible. Creating a new waveform with the same name as the predefined waveform is not possible.
<b>Group</b>	Waveform
<b>Syntax</b>	WLIST:WAveform:PREDefined? <wfm_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<wfm_name>::=<string>
<b>Returns</b>	0   1 where '0' means FALSE and '1' means TRUE
<b>Example</b>	WLIST:WAveform:PREDefined? "SINE" Might return 1 indicating that it is a predefined waveform.

**Table 213: WLIST:WAveform:PREDefined?**

<b>Command</b>	WLSt:WAveform:TYPE? (Query Only)
<b>Description</b>	This query returns if the waveform is analog or digital.
<b>Group</b>	Waveform
<b>Syntax</b>	WLSt:WAveform:TYPE? <wfm_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<wfm_name>::=<string>
<b>Returns</b>	DIGItals   ANAlog
<b>Example</b>	WLSt:WAveform:TYPE? "Ramp1000" Might return ANAlog.

Table 214: WLSt:WAveform:TYPE?

## 6.17 MULTI INSTRUMENT GROUP COMMANDS

The multi instrument synchronization is available on 8 channel models only.

The following commands have effect on 8 channel models only.

<b>Command</b>	MIM:CAPTure (No Query Form)
<b>Description</b>	This command captures all slave instruments connected to the master in which the command is sent.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:CAPTure
<b>Related Commands</b>	MIM:RELEASE
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	MIM:CAPTure This command sent on a master instrument, captures the connected slave instruments.

**Table 215:MIM:CAPTure**

<b>Command</b>	MIM:ID? (Query Only)
<b>Description</b>	This query command allows to identify the instrument of a chain. The instrument returns its number in the chain starting from the master that is 0.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:ID?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<NR1>
<b>Example</b>	MIM:ID? Might return 1 indicating the first slave of the chain.

**Table 216: MIM:ID**

<b>Command</b>	MIM:CAPTUREd? (Query Only)
<b>Description</b>	This query returns whether an instrument is captured by a master.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:CAPTUREd?
<b>Related Commands</b>	None
<b>Arguments</b>	None

<b>Returns</b>	0   1 where '0' means FALSE and '1' means TRUE
<b>Example</b>	MIM:CAPTured? Might return 1. Might return 1 indicating that the instrument has been captured by a master.

**Table 217: MIM:CAPTured**

<b>Command</b>	MIM:FORward? (Query Only)
<b>Description</b>	This query returns whether another instrument is connected to the "Synch Out" port of this instrument.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:FORward?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0   1 where '0' means FALSE and '1' means TRUE
<b>Example</b>	MIM:FORward? Might return 1. 1 indicates that another instrument is present and ready to be captured.

**Table 218: MIM:FORward**

<b>Command</b>	MIM:NUMBER? (Query Only)
<b>Description</b>	This query returns the number of captured instruments.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:NUMBER?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<value> ::= <NR1> is the number of captured instrument.
<b>Example</b>	MIM:NUMBER? Might return 2. That indicates that the instrument is master and it captured 2 other instruments.

**Table 219: MIM:NUMBER**

<b>Command</b>	MIM:SLAve? (Query Only)
<b>Description</b>	This query returns whether an instrument is slave or master. If it returns 1 it indicates that there is another instrument connected to the "Sync In" port, but it doesn't mean that the slave is captured.
<b>Group</b>	Multi Instrument

<b>Syntax</b>	MIM:SLAve?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0 1 where '0' means FALSE and '1' means TRUE
<b>Example</b>	<p>MIM:SLAve?</p> <p>Might return 1.</p> <p>1 indicates that the instrument has another instrument connected to the "Sync In" port.</p>

**Table 220: MIM:SLAve**

<b>Command</b>	MIM:RELEASE (No Query Form)
<b>Description</b>	This command sent on the master of a chain releases all captured instruments.
<b>Group</b>	Multi Instrument
<b>Syntax</b>	MIM:RELEASE
<b>Related Commands</b>	MIM:CAPTURE
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	<p>MIM:RELEASE</p> <p>This command sent on a master instrument releases the captured slave instruments.</p>

**Table 221: MIM:RELEASE**

## 7. COMMAND ERRORS

Command errors are returned when there is a syntax error in the command.

Error code	Error message
<b>-399</b>	Queue Overflow
<b>-398</b>	System Error
<b>-397</b>	No channels available
<b>-396</b>	Error to parsing waveform block data
<b>-395</b>	Waveform not found or not defined
<b>-394</b>	Sequencer not defined or incorrect data
<b>-393</b>	Waveform definition error
<b>-392</b>	Waveform out of range
<b>-391</b>	License option error
<b>-390</b>	Invalid run mode
<b>-389</b>	Subsequence error
<b>-388</b>	File Error
<b>-387</b>	Out of range error
<b>-386</b>	Application error
<b>-385</b>	Data type error
<b>-384</b>	Diagnostic error
<b>-383</b>	Calibration error
<b>-382</b>	Error on loading setting into the instrument
<b>-381</b>	Error on writing the serial number
<b>-380</b>	Error on reading the status of the digital input pins
<b>-379</b>	Waveform length different between channels in one sequencer/subsequencer entry
<b>-378</b>	Unable to set the Attenuation Value; if the Attenuation value is greater than 20dB, the Vocm value must be in the following range: +-250mV
<b>-377</b>	Predefined Waveform Error (it is not possible to delete or create a predefined waveform)
<b>-376</b>	Waveform Granularity Error
<b>-375</b>	Digital port disabled error: the digital port is disabled.
<b>-374</b>	The start operation is failed
<b>-373</b>	The stop operation is failed
<b>-372</b>	The trigger operation is failed

<b>-371</b>	Load configuration error
<b>-370</b>	Import configuration error
<b>-369</b>	Save configuration error
<b>-368</b>	A configuration with the same name is already present
<b>-367</b>	Delete configuration error
<b>-366</b>	The configuration is locked
<b>-365</b>	The parameter is disabled
<b>-364</b>	No digitals programmed
<b>-363</b>	Wrong format
<b>-362</b>	The device is in running status
<b>-361</b>	Load license error
<b>-360</b>	Lock unlock license error
<b>-359</b>	Copy configuration error
<b>-358</b>	Delete waveform error
<b>-357</b>	No valid MSUS
<b>-356</b>	No valid folder
<b>-355</b>	No valid file
<b>-354</b>	IO file error
<b>-353</b>	File system operation error
<b>-352</b>	Start index error
<b>-351</b>	Size error
<b>-350</b>	Load waveform error
<b>-349</b>	Waveform already present error
<b>-348</b>	Wrong path error
<b>-347</b>	Predefined waveform
<b>-346</b>	Wrong block data
<b>-345</b>	Sequencer memory overflow
<b>-344</b>	No license installed
<b>-343</b>	Wrong waveform name
<b>-342</b>	The device is captured from the master device
<b>-341</b>	Multi Instrument management error
<b>0</b>	No error

<b>5</b>	DESIGN ERROR: Too many numeric suffices in Command Spec
<b>10</b>	No Input Command to parse
<b>14</b>	Numeric suffix is invalid value
<b>16</b>	Invalid value in numeric or channel list, e.g. out of range
<b>17</b>	Invalid number of dimensions in a channel list
<b>20</b>	Parameter of type Numeric Value overflowed its storage
<b>30</b>	Wrong units for parameter
<b>40</b>	Wrong type of parameter(s)
<b>50</b>	Wrong number of parameters
<b>60</b>	Unmatched quotation mark (single/double) in parameters
<b>65</b>	Unmatched bracket
<b>70</b>	Command keywords were not recognized
<b>200</b>	No entry in list to retrieve (number list or channel list)
<b>210</b>	Too many dimensions in entry to be returned in parameters
<b>220</b>	; plus End of line commands

**Table 222: Command Errors**

## 8. PREDEFINED WAVEFORMS

<b>SINE</b>	Sine waveform, 16384 samples, analog, normalized
<b>RAMP</b>	Ramp waveform, 16384 samples, analog, normalized
<b>SQUARE</b>	Square waveform, 16384 samples, analog, normalized
<b>SYNC</b>	Sync waveform, 16384 samples, analog, normalized
<b>DC</b>	DC level waveform, 16384 samples, analog, normalized
<b>GAUSSIAN</b>	Gaussian waveform, 16384 samples, analog, normalized
<b>LORENTZ</b>	Lorentz waveform, 16384 samples, analog, normalized
<b>HAVERSINE</b>	Haversine waveform, 16384 samples, analog, normalized
<b>EXP_RISE</b>	Exponential rise waveform, 16384 samples, analog, normalized
<b>EXP_DECAY</b>	Exponential decay waveform, 16384 samples, analog, normalized
<b>ZERO</b>	All Zeros, 16384 samples, digital
<b>ONE</b>	All Ones, 16384 samples, digital
<b>COUNTER</b>	Counter, 256 samples, digital
<b>CLOCK</b>	Clock, 16 samples, digital

**Table 223: Predefined Waveforms**

## 9. REMOTE CONTROL

You can connect your instrument to a network for printing, file sharing, and Internet access, among other functions. Consult with your network administrator and use the standard Windows utilities to configure the instrument for your network.

The instrument can be controlled using VXI-11 (LAN) protocol. It allows you to control the instrument remotely by using SCPI commands. Please refer to the Arb AWG-3000 programmer manual for a complete description about all available commands. You can follow the next steps to communicate with your AWG-3000 Series instrument:


### 9.1 PREREQUISITE

#### NI-VISA

VISA provides the programming interface between the hardware and development environments such as Visual Studio .NET, LabVIEW, LabWindows/CVI, Measurement Studio for Microsoft Visual Studio and MatLab. NI-VISA is the National Instruments implementation of the VISA I/O standard. NI-VISA includes software libraries, interactive utilities such as NI I/O Trace and the VISA Interactive Control, and configuration programs through Measurement & Automation Explorer for all your development needs.


1. Connect your LAN cable to the instrument.
2. On the Client-PC you must install the latest NIVISA package that you can find here  
<https://www.ni.com/it-it/support/downloads/drivers/download.ni-visa.html>

### 3. Launch the NI-MAX tool on the Client-PC

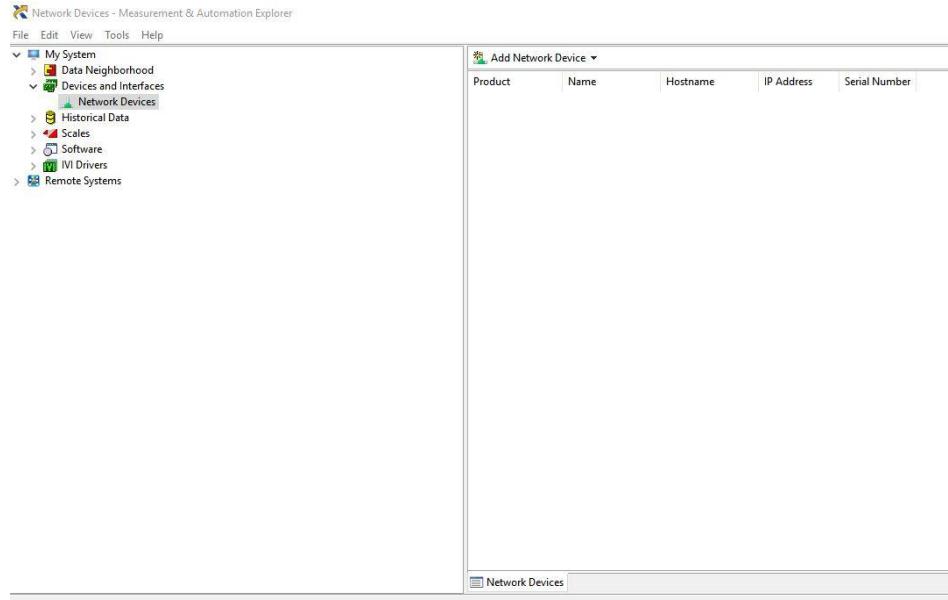


Press Add Network Device → VISA TCP/IP Resource...


### 4. Select Auto-detect of LAN Instrument

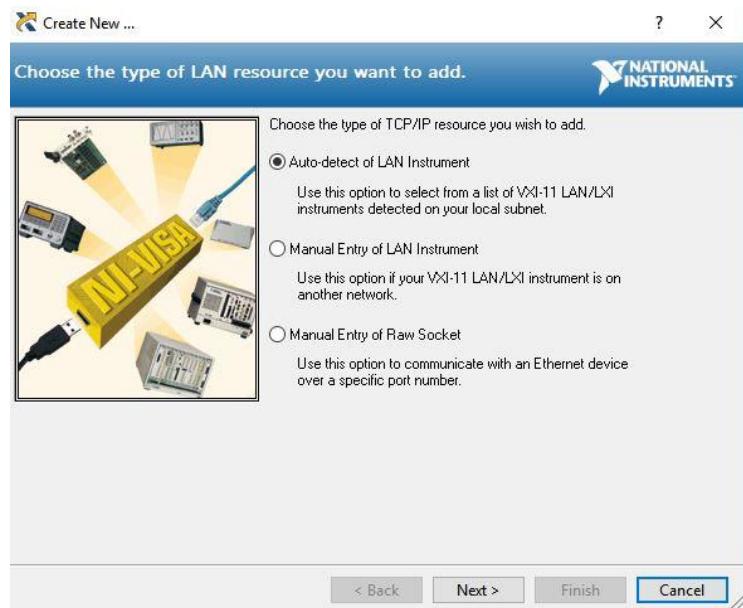


5. The panel will retrieve the discovered instruments on the LAN network, you should select the AWG3000X series one.

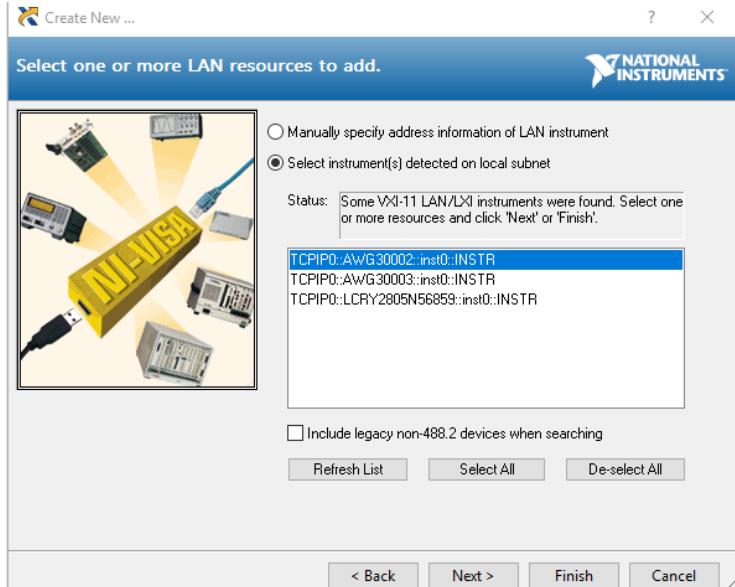


6. Specify an Alias for the selected resource

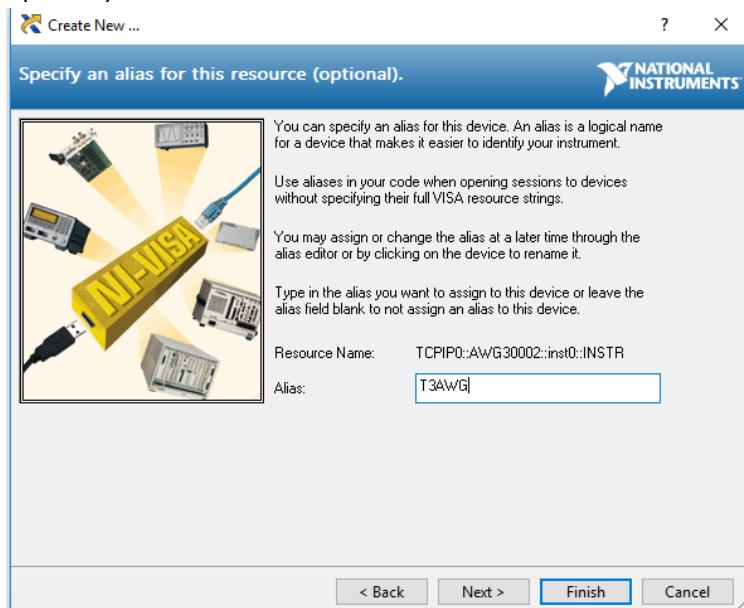


7. Press Finish

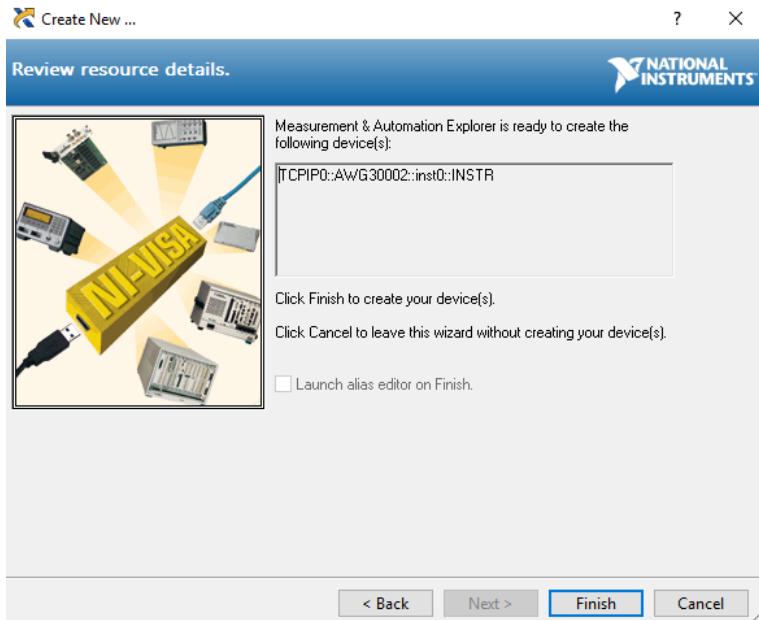

8. The T3AWG resource will be available in the Network Devices list

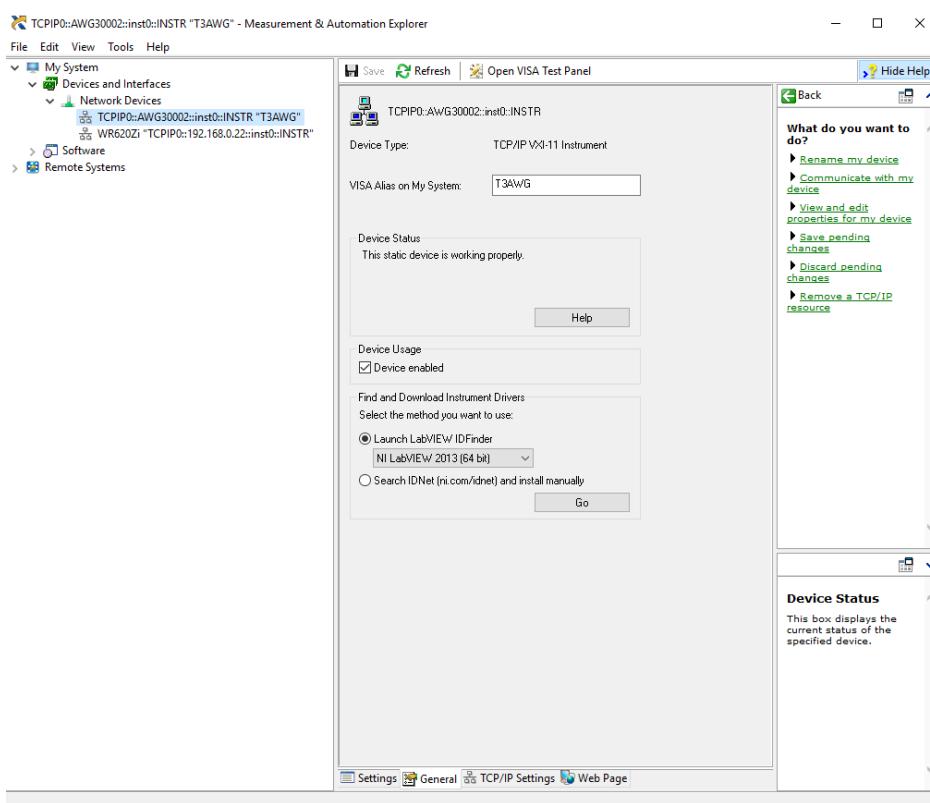


9. Now you can use send the SCPI commands to the T3AWG resource using the NI Visa Test Panel or the AT-Instrument-Communicator

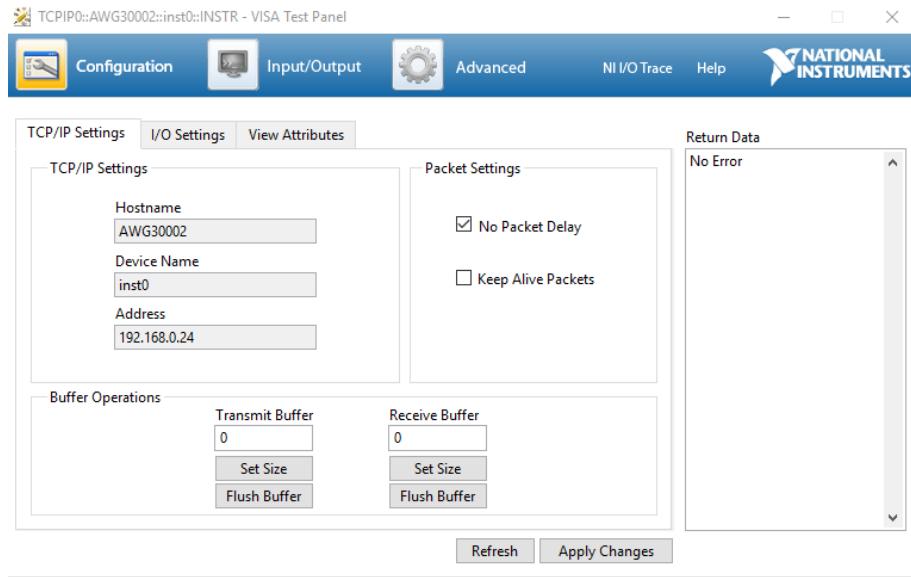

10. On the Client-PC (IP Address) or AWG instrument (localhost), launch the AT-Instrument-Communicator tool

## 9.1.1 AT Instrument Communicator

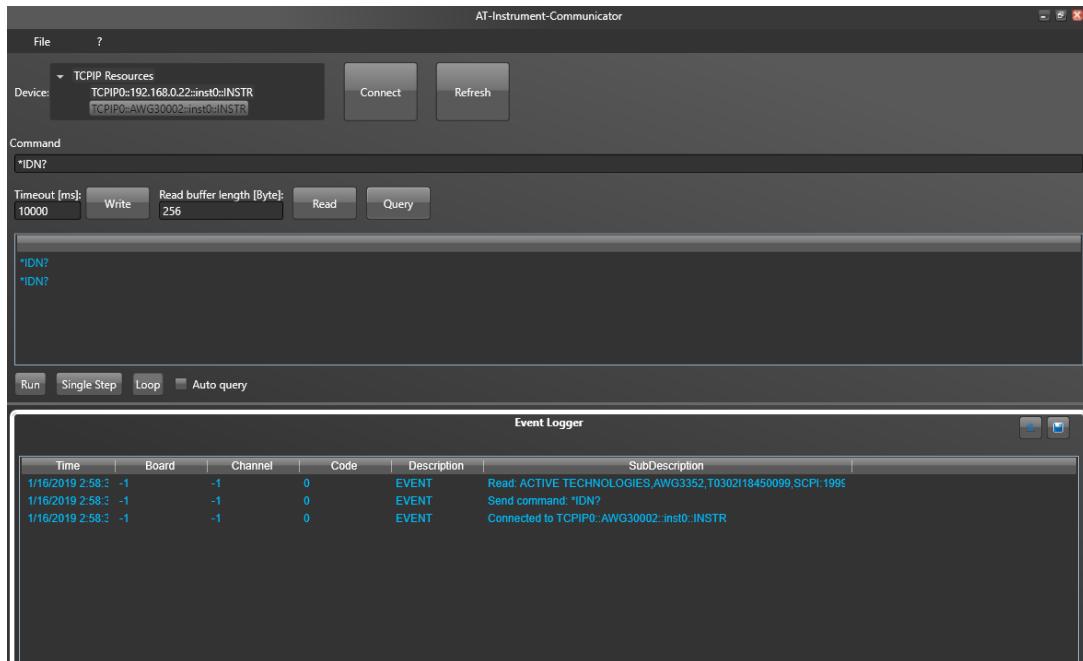


The AT-Instrument-Communicator software is a client-side component tool that uses NI-VISA on each remote PC, you must install a copy of NIVISA to make use of this client-side component (please follow the Prerequisite steps).

1. On the Client-PC launch the *AT Instrument Communicator* setup you can find in the folder “SDK\_TRUEARB\_AWG\_3000” and install the software.
2. Select the AWG3000X resource on the Device list
3. Press the Connect button
4. If the instrument connection will be established, the SCPI command button will be enabled.
5. Write \*IDN? in the command
6. Press the Query button

7. In the Event Logger list, the instrument should respond like this:  
ACTIVE TECHNOLOGIES,T3AWG3352,T0302I000001,SCPI:1999.0,SV:AWG.3.2.9 where  
T0302I000001 is the serial number, SCPI:1999.0 is the SCPI command version and  
SV:AWG.3.2.9 is the Application and Software Version.
8. A command script is a list of SCPI commands (one command for each line) saved in a  
txt file; you can send a command script using the File → Load Script menu item.

## 9.2 NI LABVIEW EXAMPLES

The LabView examples require at least LabView 2013 64 bit version, you should copy SDK\_TRUEARB\_T3AWG3K\_Teledyne Test Tools folder in ...\\LabVIEW 2013\\instr.lib folder on your computer and open the file Active Technologies AWG3000.lvproj.

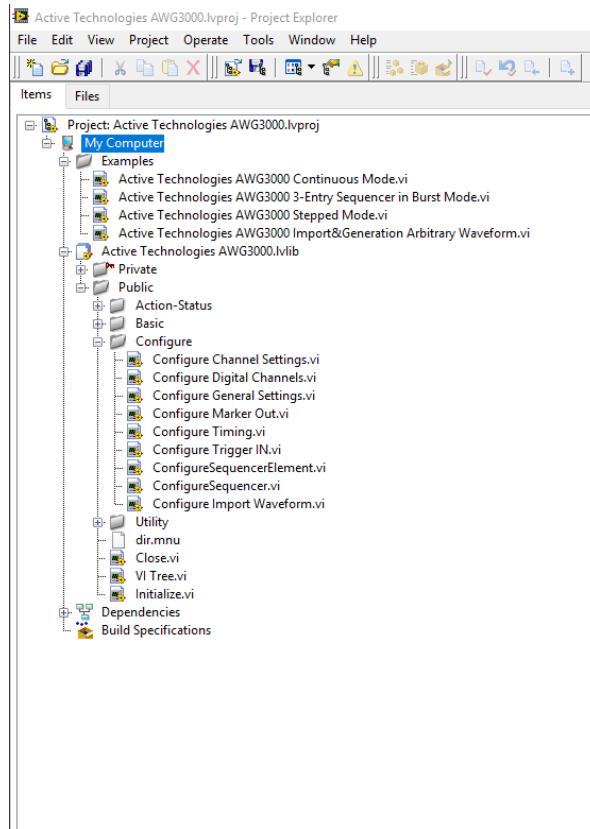

The LabView project contains several Vis that control the basic instrument features and four examples located in the folder Examples.

Note: for proper usage of Labview's Vis it's necessary that decimal symbol separator is properly set on your PC.

So please check that the Dot symbol “.” is set in *Decimal Symbol* field that you can find:

### In Windows 10


1. From the **Start** button click **Control Panel**.
2. Click **Region**.
3. On the **Formats** tab click the **Additional Settings** button.

## In Windows 7

1. From the **Start** button click **Control Panel**.
2. Click **Regional and Language Options**.
3. On the **Formats** tab, under **Current format**, click **Customize this format**.

### 9.2.1 CONTINUOUS MODE

Double click on the project tree to launch the Active Technologies AWG3000 Continuous Mode.vi example

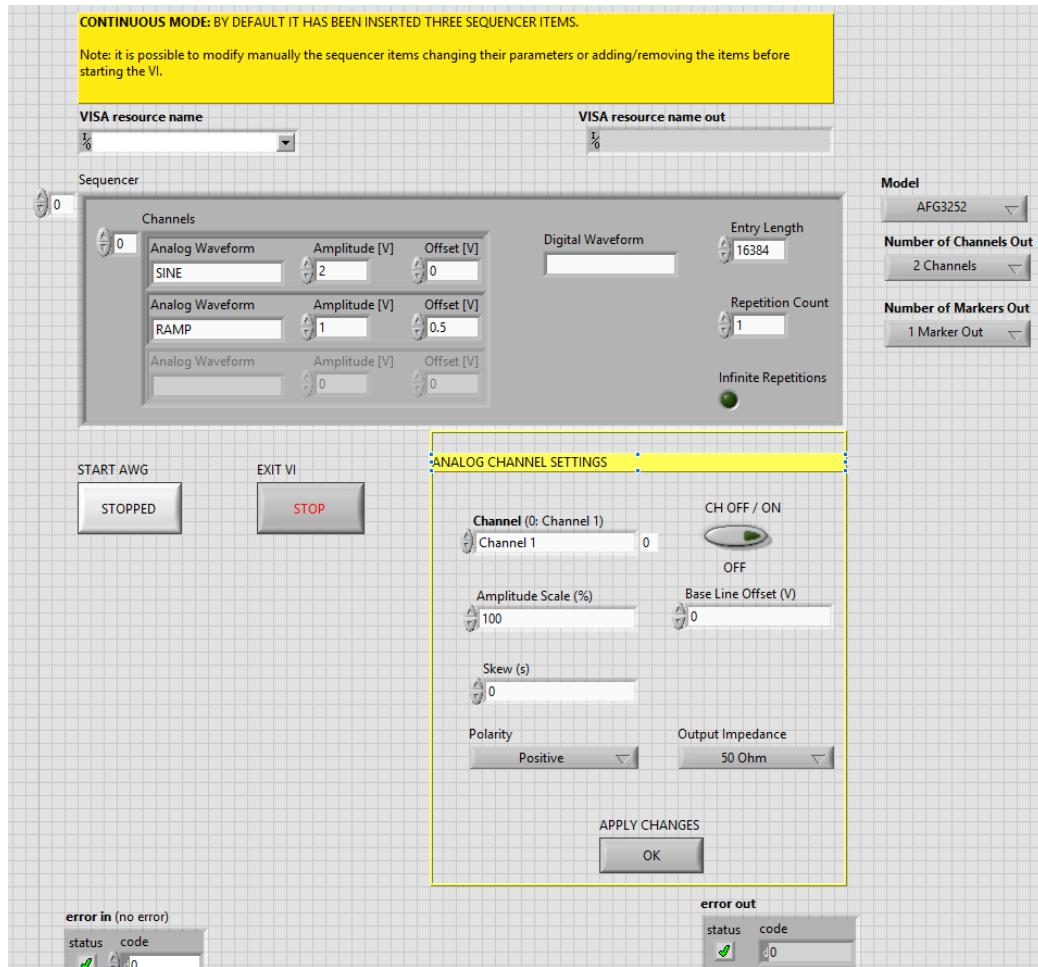

This example generates a sequence of waveforms in Continuous mode; the sequencer by default is made of three entries and it is loaded as follows:

	<b>Entry 1 – Length 16384, Rep. 1</b>	<b>Entry 2 – Length 16384, Rep. 2</b>	<b>Entry 3 – Length 16384, Rep. 3</b>
CH1	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 3V, Offset 0V	Lorentz, Amp. 4V, Offset 0V
CH2	Ramp, Amp. 1V, Offset 0.5V	Sync, Amp. 3V, Offset 0V	Lorentz, Amp. 4V, Offset 0V


Before running the VI you have to select the AWG-3000 resource in the VISA resource name control.

- Run the VI and press the “START AWG” button to start the generation.
- The Analog Channel Settings section lets you to change on the fly the Amplitude Scale, the Base Line Offset, the Skew, the Polarity and the Output Impedance parameters. Select the Channel and press the Apply Changes button to confirm the changes.
- You can press the CH OFF/ON button to enable or disable the analog channel.

The entire sequence will be repeated continuously until you press again the “START AWG” button.

## 9.2.2 BURST MODE

Double click on the project tree to launch the *Active Technologies AWG3000 3-Entry Sequencer in Burst mode.vi* example.

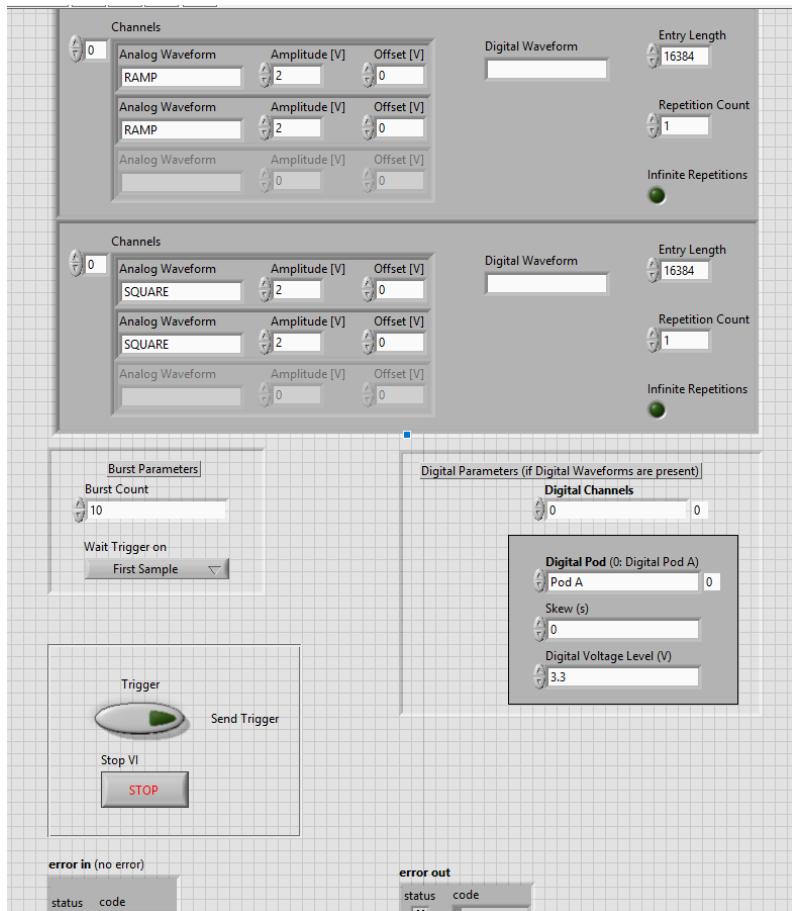

This example generates a sequence of waveforms in Burst Mode.  
The sequencer by default is loaded as follows:

	<b>Entry 1 – Length 16384, Rep. 1</b>	<b>Entry 2 – Length 16384, Rep. 1</b>	<b>Entry 3 – Length 16384, Rep. 1</b>
CH1	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Square, Amp. 2V, Offset 0V

CH2	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Square, Amp. 2V, Offset 0V
-----	--------------------------	--------------------------	----------------------------

In the “Burst Parameters” section, you can change the number of burst (Burst Count) and the Wait Trigger On parameter.


If you load Digital Waveforms in the sequencer, in the “Digital Parameters” section, you can select the number of Digital channels, the Digital Pod, the Skew and the Digital Voltage Level.

Run the VI to initialize the instrument and load the default parameters into the instrument; the Send Trigger button starts the waveform sequence burst.

Press the STOP button to stop the waveform generation and the VI.

### 9.2.3 STEPPED MODE

Double click on the project tree to launch the Active Technologies AWG3000 Stepped Mode.vi example

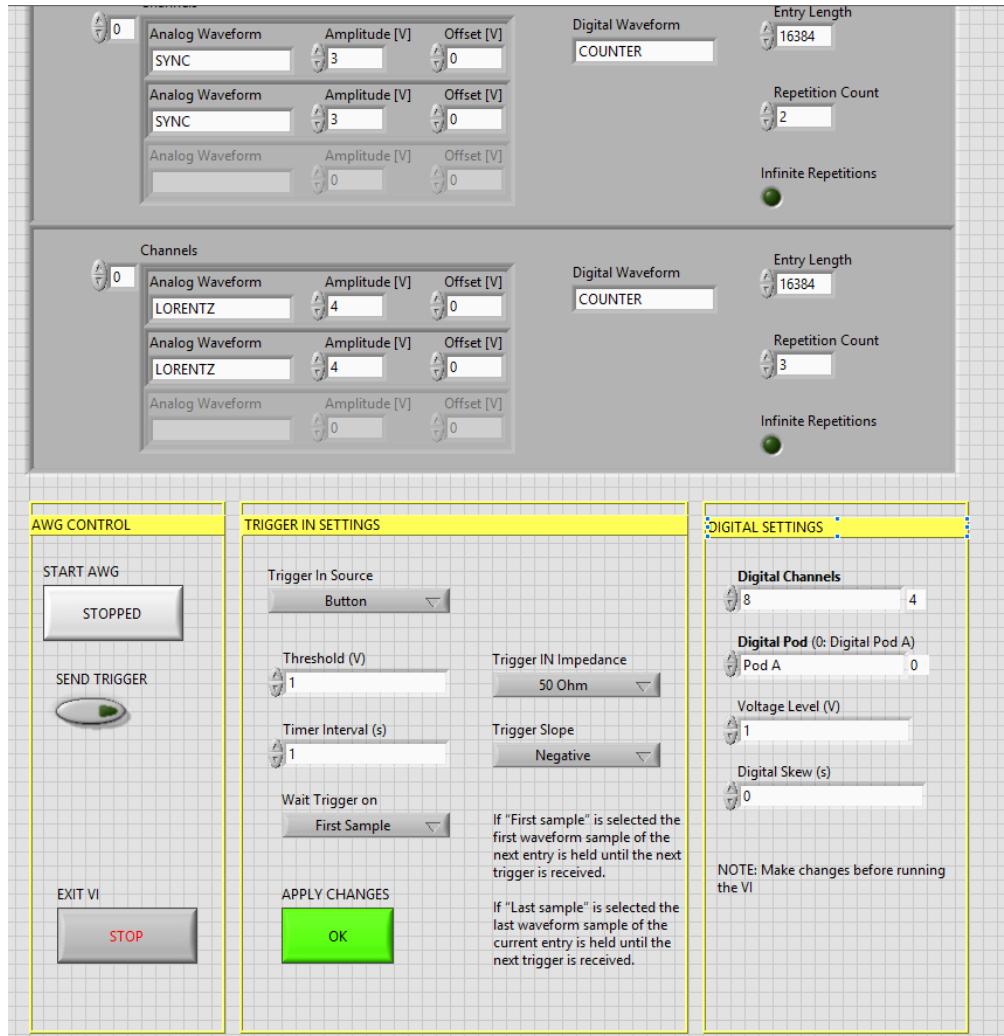

This example generates a sequence of waveforms in Stepped Mode.

In this mode after pressing the RUN/STOP button each entry waits for a trigger event before its execution. The waveform of the entry will loop as written in the entry repetition parameter.

The sequencer by default is loaded as follows:

	<b>Entry 1 – Length 16384, Rep. 1</b>	<b>Entry 2 – Length 16384, Rep. 2</b>	<b>Entry 3 – Length 16384, Rep. 3</b>
CH1	Sine, Amp. 2V, Offset 0V	Sync, Amp. 3V, Offset 0V	Lorentz, Amp. 4V, Offset 0V
CH2	Exp. Rise, Amp. 2V, Offset 0V	Sync, Amp. 3V, Offset 0V	Lorentz, Amp. 4V, Offset 0V
DIG. WAV.	COUNTER	COUNTER	COUNTER

Before running the VI you can configure in the “Digital Settings” the number of digital channels, the digital pod voltage level and the digital skew.


1. Run the VI: by default the instrument will receive the trigger from the front panel button
2. Press the “START AWG” button to run the AWG
3. Press the “SEND TRIGGER” button to send a software trigger

In the “Trigger IN Settings”, you can configure the Trigger In Source, the Threshold, the Trigger IN impedance, the Timer Interval, the Trigger Slope and the Wait Trigger On Parameter.

Stop the instrument and then press the "APPLY CHANGES" button to confirm changes on the TRIGGER IN settings.

## 9.2.4 ADVANCED MODE

Double click on the project tree to launch the Active Technologies AWG3000 Advanced Mode.vi example

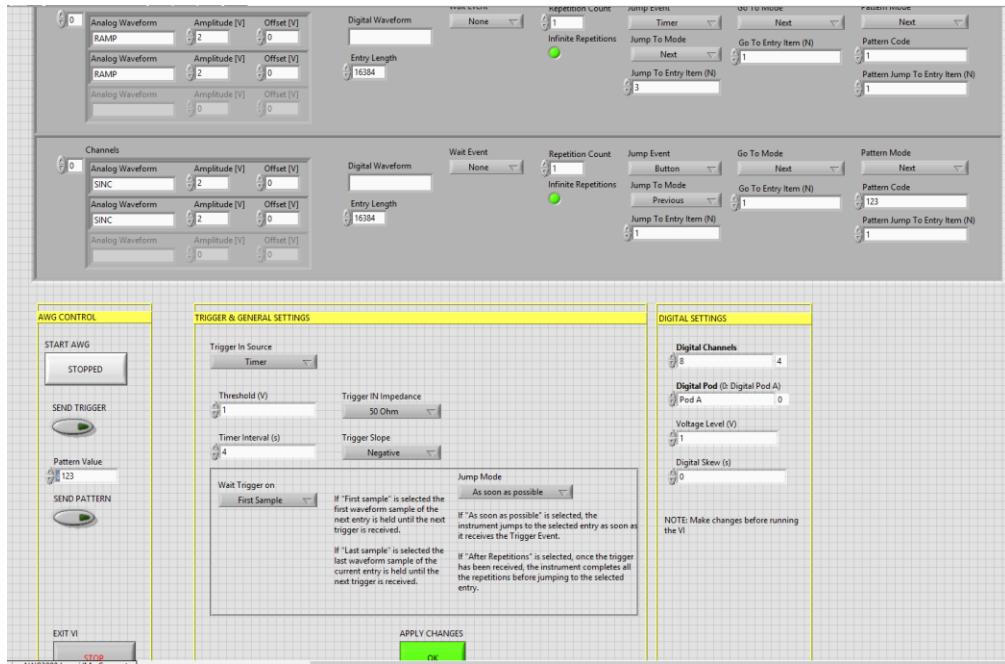

This example generates a sequence of waveforms in Advanced Mode.

In this mode the execution of the sequence can be changed by using conditional and unconditional jumps (JUMPTO and GOTO commands) and dynamic jumps (PATTERN JUMP commands).

The sequencer by default is loaded as follows:

<b>Entry 1 – Length 16384 -</b> <b>Wait Event Button   Rep. 100</b> <b>  Infinite Repetitions Off  </b> <b>Jump Event None   Jump To</b> <b>Mode Next Jump to Entry</b> <b>Item 1 Go To Mode Next  </b> <b>Go To Entry Item 1   Pattern</b> <b>Mode Next   Pattern Code</b>	<b>Entry 2 – Length 16384 -</b> <b>Wait Event None   Rep. 1</b> <b>  Infinite Repetitions On  </b> <b>Jump Event Timer   Jump To</b> <b>Mode Next Jump to Entry</b> <b>Item 3 Go To Mode Next  </b> <b>Go To Entry Item 1   Pattern</b> <b>Mode Next   Pattern Code</b>	<b>Entry 3 – Length 16384 –</b> <b>Wait Event None   Rep.</b> <b>1   Infinite Repetitions</b> <b>On  </b> <b>Jump Event Button  </b> <b>Jump To Mode</b> <b>Previous   Jump to Entry</b> <b>Item 1 Go To Mode</b> <b>Next   Go To Entry Item</b>
--	--	--

	<b>1   Pattern Jump To Entry Item 1</b>	<b>1   Pattern Jump To Entry Item 1</b>	<b>1   Pattern Mode Next   Pattern Code 123   Pattern Jump To Entry Item 1</b>
CH1	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Sinc, Amp. 2V, Offset 0V
CH2	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Sinc, Amp. 2V, Offset 0V

Before running the VI you can configure in the “Digital Settings” the number of digital channels, the digital pod voltage level and the digital skew. You can also add a Digital Waveform to the sequencer.


4. Run the VI. By default the instrument will receive the trigger from the front panel button.
5. Press the “START AWG” button to run the AWG.
6. You can press the “SEND TRIGGER” button to send a software trigger, you can press the “SEND PATTERN” button to send the pattern code value.
7. By default the execution of the sequencer is the following one: press the SEND TRIGGER button to start the waveform repetitions of the first entry.
8. On the second entry, the instrument waits for the timer event before executing the JUMP to the third entry.
9. On the third entry, the instrument can accept the trigger button (software trigger) as Jump Event to the Previous Entry or the PATTERN code value to Jump to the first entry of the sequencer: you can press the SEND TRIGGER button or the SEND PATTERN button to change the execution order of the waveform sequence.

In the “Trigger & General Settings”, you can configure the Trigger In Source, the Threshold, the Trigger IN impedance, the Timer Interval, the Trigger Slope, the Wait Trigger On Parameter and the Jump Mode parameter.

Stop the instrument and then press the "APPLY CHANGES" button to confirm changes on the TRIGGER & GENERAL settings.

## 9.2.5 IMPORT AN ARBITRARY WAVEFORM GENERATION

This example lets you to create analog or digital waveforms, import them in the Waveform List and then load the sequencer with the generated waveforms. By default the instrument is set in Continuous mode.

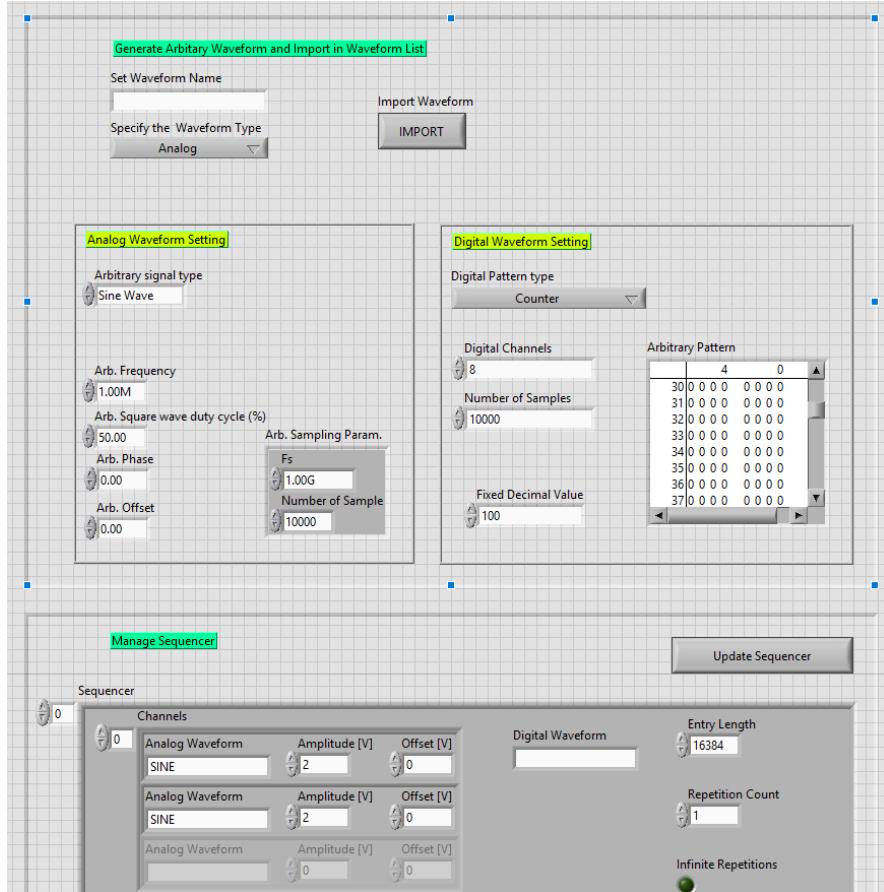


In the Analog Waveform Setting section you have different parameters to set the analog waveform: you can select the arbitrary signal type between Sine, Triangle, Square and Sawtooth waveform, you can change the frequency, the duty cycle, the phase and the offset. Moreover, you can set the sampling rate and the number of samples.

In the Digital Waveform Setting section you have different parameters to set the digital waveform; in the Digital Pattern type dropdown list you can select between a counter, a random number, a fixed value or an arbitrary pattern.

When you select “arbitrary pattern”, you can set in the Arbitrary Pattern table the samples of the waveform: the row is the sample number and the column is the digital line.

The Digital Channels and the Number of Samples parameters define the number of digital lines available in the instrument and the number of samples of the digital waveform.

The Manage Sequencer section allows you to configure the sequencer with predefined or arbitrary waveforms.

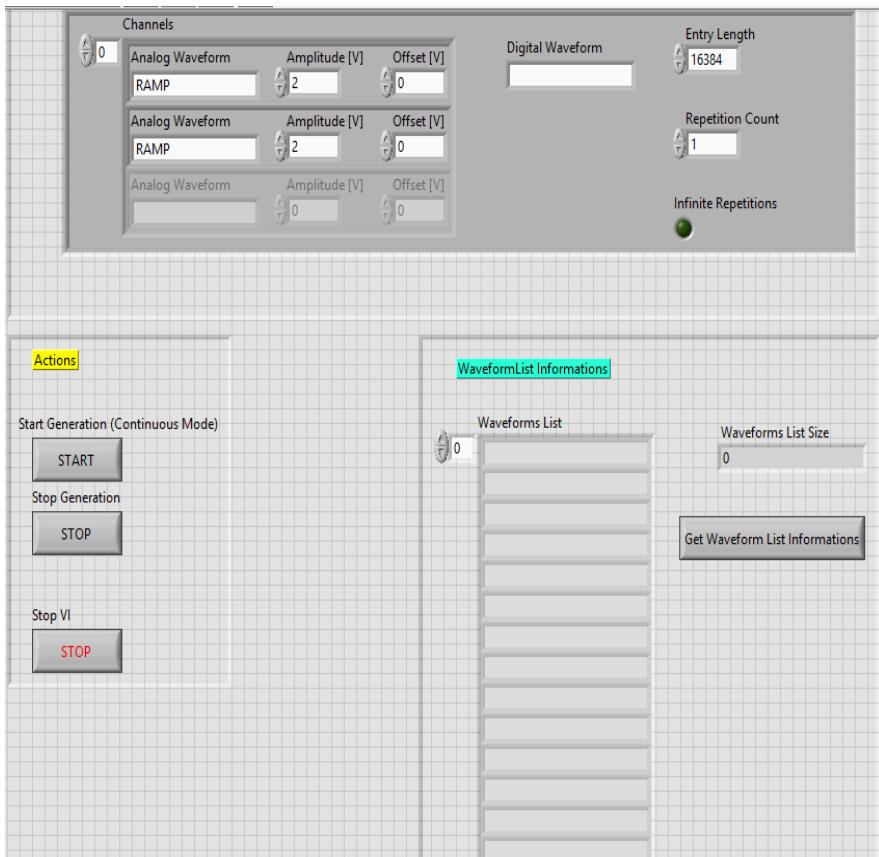

The “WaveformList Informations” section allows you to know the names of the available predefined and imported waveforms in the instrument.

The following steps describe how to create and import an analog/digital waveform:

1. Run the VI
2. In the “Set Waveform Name” control write SINE\_120MHZ
3. Set Analog in the “Specify the Waveform Type” dropdown list

4. In the Analog Waveform Setting section set Sine Wave as signal type, 120 MHz in the Arb. Frequency, 1 GHz as Fs (sampling rate) and 12000 as number of samples.
5. Press the Import button
6. In the “Set Waveform Name” control write RAND\_12000
7. Set Digitals in the “Specify the Waveform Type” dropdown list
8. In the Digital Waveform Setting section select Random in the Digital Pattern Type, set 8 Digital Channels and 12000 in the Number of Samples Parameter
9. Press the Import button
10. Press the button “Get Waveform List Informations” and in the waveform list it will appear SINE\_120MHZ and RAND\_12000.
11. The sequencer by default will be loaded as:

	<b>Entry 1 – Length 16384, Rep. 1</b>	<b>Entry 2 – Length 16384, Rep. 1</b>	<b>Entry 3 – Length 16384, Rep. 1</b>
CH1	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Square, Amp. 2V, Offset 0V
CH2	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	Square, Amp. 2V, Offset 0V
DIG.WAV.			

12. Replace the third entry with the imported ones

	<b>Entry 1 – Length 16384, Rep. 1</b>	<b>Entry 2 – Length 16384, Rep. 1</b>	<b>Entry 3 – Length 12000, Rep. 1</b>
CH1	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	SINE_120MHZ, Amp. 2V, Offset 0V
CH2	Sine, Amp. 2V, Offset 0V	Ramp, Amp. 2V, Offset 0V	SINE_120MHZ, Amp. 2V, Offset 0V
DIG.WAV.	ONE	ZERO	RAND_12000

13. Press the Update Sequencer button to load the new sequencer

14. Press the START button to run the AWG

## 9.3 SCRIPT EXAMPLES

The scripts are contained in the folder “Sample Scripts”

### 9.3.1 CONTINUOUS MODE

```
*CLS
*IDN?
*RST
AWGControl:INCreasing INTERpolation
AWGControl:DECReasing DECIMation
AWGControl:RMODE CONTinuous
DISPlay:UNIT:VOLT AMPLitudeoff
SEQuence:LENGth 3
SEQuence:ELEM1:WAVEform1 "SINE"
SEQuence:ELEM1:AMPlitude1 2.000000
SEQuence:ELEM1:OFFset1 0.000000
SEQuence:ELEM1:WAVEform2 "RAMP"
SEQuence:ELEM1:AMPlitude2 1.000000
SEQuence:ELEM1:OFFset2 0.500000
SEQuence:ELEM1:LENGth 16384
SEQuence:ELEM1:LOOP:COUNT 1
SEQuence:ELEM2:WAVEform1 "RAMP"
SEQuence:ELEM2:AMPlitude1 3.000000
SEQuence:ELEM2:OFFset1 0.000000
SEQuence:ELEM2:WAVEform2 "SYNC"
SEQuence:ELEM2:AMPlitude2 3.000000
SEQuence:ELEM2:OFFset2 0.000000
SEQuence:ELEM2:LENGth 16384
SEQuence:ELEM2:LOOP:COUNT 2
SEQuence:ELEM3:WAVEform1 "LORENTZ"
SEQuence:ELEM3:AMPlitude1 4.000000
SEQuence:ELEM3:OFFset1 0.000000
SEQuence:ELEM3:WAVEform2 "LORENTZ"
SEQuence:ELEM3:AMPlitude2 4.000000
SEQuence:ELEM3:OFFset2 0.000000
SEQuence:ELEM3:LENGth 16384
SEQuence:ELEM3:LOOP:COUNT 3
AWGControl:CONFigure:CNUMber?
OUTPut1:STATe ON
OUTPut2:STATe ON
AWGControl:RUN
```

### 9.3.2 STEPPED MODE

Note: the trigger is set as manual; this script includes also the digital lines

```
*CLS
*IDN?
*RST
AWGControl:CONFigure:CNUMber?
AWGControl:RMODe STEPped
AWGControl:WAITstate FIRST
DIGItals:NUMber 8
DIGItals:LEVel1 1.000000
DIGItals:SKEW1 0.000000
DIGItals:STATe ON
SEQuence:LENGth 3
DISPlay:UNIT:VOLT AMPLitudeoff
SEQuence:ELEM1:WAVeform1 "SINE"
SEQuence:ELEM1:AMPlitude1 2.000000
SEQuence:ELEM1:OFFset1 0.000000
SEQuence:ELEM1:WAVeform2 "EXP_RISE"
SEQuence:ELEM1:AMPlitude2 2.000000
SEQuence:ELEM1:OFFset2 0.000000
SEQuence:ELEM1:WAVeform3 "COUNTER"
SEQuence:ELEM1:LENGth 16384
SEQuence:ELEM1:LOOP:COUNT 1
SEQuence:ELEM2:WAVeform1 "SYNC"
SEQuence:ELEM2:AMPlitude1 3.000000
SEQuence:ELEM2:OFFset1 0.000000
SEQuence:ELEM2:WAVeform2 "SYNC"
SEQuence:ELEM2:AMPlitude2 3.000000
SEQuence:ELEM2:OFFset2 0.000000
SEQuence:ELEM2:WAVeform3 "COUNTER"
SEQuence:ELEM2:LENGth 16384
SEQuence:ELEM2:LOOP:COUNT 2
SEQuence:ELEM3:WAVeform1 "LORENTZ"
SEQuence:ELEM3:AMPlitude1 4.000000
SEQuence:ELEM3:OFFset1 0.000000
SEQuence:ELEM3:WAVeform2 "LORENTZ"
SEQuence:ELEM3:AMPlitude2 4.000000
SEQuence:ELEM3:OFFset2 0.000000
SEQuence:ELEM3:WAVeform3 "COUNTER"
SEQuence:ELEM3:LOOP:COUNT 3
TRIGger:SOURce MAN
```

```
OUTPut1:STATe ON
OUTPut2:STATe ON
AWGControl:RUN
*TRG
```

### 9.3.3 IMPORT ARBITRARY

1. Before running this script, please copy the folder "Example\_Wave\_TXT" into the instrument folder C:\Users\AWG3000\Pictures\Saved Pictures\
2. The 10000\_Sample\_Analog\_Sine\_Wave.txt contains a set of analog sine waves made of 10000 samples. The 10000\_Sample\_Digital\_Random\_Pattern.txt is a digital random pattern made of 10000 samples.
3. The aim of this example is to import them in the sequencer and run the instrument in Continuous mode.

```
*CLS
*IDN?
*RST
AWGControl:CONFigure:CNUMber?
AWGControl:RMODE CONTinuous
DISPLAY:UNIT:VOLT AMPLitudeoff
DIGItals:NUMber 8
DIGItals:LEVel1 3.000000
DIGItals:SKEW1 0.000000
DIGItals:STATe ON
WLst:WAveform:IMPort
"Sine_10000","\\Example_Wave_TXT\\10000_Sample_Analog_Sine_Wave.txt",ANALog
WLst:WAveform:IMPort "Digital_10000",
"\\"\\Example_Wave_TXT\\10000_Sample_Digital_Random_Pattern.txt",DIGItal
SEQUence:LENGTH 1
SEQUence:ELEM1:WAveform1 "Sine_10000"
SEQUence:ELEM1:AMPlitude1 2.000000
SEQUence:ELEM1:OFFset1 0.000000
SEQUence:ELEM1:WAveform2 "Sine_10000"
SEQUence:ELEM1:AMPlitude2 2.000000
SEQUence:ELEM1:OFFset2 0.000000
SEQUence:ELEM1:WAveform3 "Digital_10000"
SEQUence:ELEM1:LENGTH 10000
SEQUence:ELEM1:LOOP:COUNT 1
OUTPut1:STATe ON
OUTPut2:STATe ON
AWGControl:RUN
```

### 9.3.4 ADVANCED MODE

```
*CLS
*IDN?
*RST
AWGControl:INCreasing INTERpolation
AWGControl:DECreasing DECIMation
AWGControl:RMODe ADVAnced
AWGControl:WAITstate FIRST
AWGControl:JUMPMode IMMEDIATE
AWGControl:CONFigure:CNUMber?
SEQuence:LENGth 3
DISPlay:UNIT:VOLT AMPLitudeoff
SEQuence:ELEM1:WAVeform1 "SINE"
SEQuence:ELEM1:AMPlitude1 2.000000
SEQuence:ELEM1:OFFset1 0.000000
SEQuence:ELEM1:WAVeform2 "SINE"
SEQuence:ELEM1:AMPlitude2 2.000000
SEQuence:ELEM1:OFFset2 0.000000
SEQuence:ELEM1:LENGth 16384
SEQuence:ELEM1:LOOP:COUNT 100
SEQuence:ELEM1:WAITEvent MANual
SEQuence:ELEM1:JUMPEvent NONE
SEQuence:ELEM1:JUMPTOMode NEXT
SEQuence:ELEM1:JUMPTOEntry 1
SEQuence:ELEM1:GOTOMode NEXT
SEQuence:ELEM1:GOTOEntry 1
SEQuence:ELEM1:PATTERNJUMPTOMode NEXT
SEQuence:ELEM1:PATTERN 1
SEQuence:ELEM1:PATTERNJUMPTOEntry 1
DISPlay:UNIT:VOLT AMPLitudeoff
SEQuence:ELEM2:WAVeform1 "RAMP"
SEQuence:ELEM2:AMPlitude1 2.000000
SEQuence:ELEM2:OFFset1 0.000000
SEQuence:ELEM2:WAVeform2 "RAMP"
SEQuence:ELEM2:AMPlitude2 2.000000
SEQuence:ELEM2:OFFset2 0.000000
SEQuence:ELEM2:LENGth 16384
SEQuence:ELEM2:LOOP:COUNT INFinite
SEQuence:ELEM2:WAITEvent NONE
```

SEQuence:ELEM2:JUMPEvent TIMer  
SEQuence:ELEM2:JUMPTOMode NEXT  
SEQuence:ELEM2:JUMPTOEntry 3  
SEQuence:ELEM2:GOTOMode NEXT  
SEQuence:ELEM2:GOTOEntry 1  
SEQuence:ELEM2:PATTERNJUMPTOMode NEXT  
SEQuence:ELEM2:PATTERN 1  
SEQuence:ELEM2:PATTERNJUMPTOEntry 1  
DISPlay:UNIT:VOLT AMPLitudeoff  
SEQuence:ELEM3:WAveform1 "SINC"  
SEQuence:ELEM3:AMPlitude1 2.000000  
SEQuence:ELEM3:OFFset1 0.000000  
SEQuence:ELEM3:WAveform2 "SINC"  
SEQuence:ELEM3:AMPlitude2 2.000000  
SEQuence:ELEM3:OFFset2 0.000000  
SEQuence:ELEM3:LENGTH 16384  
SEQuence:ELEM3:LOOP:COUNT INFinite  
SEQuence:ELEM3:WAITEvent MANUAL  
SEQuence:ELEM3:JUMPEvent NONE  
SEQuence:ELEM3:JUMPTOMode PREVIOUS  
SEQuence:ELEM3:JUMPTOEntry 1  
SEQuence:ELEM3:GOTOMode NEXT  
SEQuence:ELEM3:GOTOEntry 1  
SEQuence:ELEM3:PATTERNJUMPTOMode NEXT  
SEQuence:ELEM3:PATTERN 123  
SEQuence:ELEM3:PATTERNJUMPTOEntry 1  
TRIGger:SOURce TIMER  
TRIGger:LEVel 1.000000  
TRIGger:SLOPe NEGative  
TRIGger:IMPedance 50Ohm  
TRIGger:TImer 4.000000  
OUTPUT1:STATe ON  
OUTPUT2:STATe ON  
AWGControl:RUN  
\*TRG  
AWGControl:DJStrobe 123